

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021822\
 Data File : VU047214.D
 Acq On : 17 Feb 2022 19:10
 Operator : SY/MD
 Sample : N1559-11DL 4X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M85DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	95	rBV	79278	91869	13.27%	1.543%
2	1.919	171	180	199	rBV	65051	91160	13.17%	1.531%
3	2.572	371	383	401	rBV	125505	204266	29.50%	3.432%
4	3.054	523	533	551	rVB2	5213	9969	1.44%	0.167%
5	4.642	1012	1027	1075	rVB	89673	275297	39.76%	4.625%
6	5.067	1143	1159	1184	rBV	122361	272850	39.41%	4.584%
7	5.729	1344	1365	1387	rBV2	235585	610625	88.19%	10.259%
8	6.253	1514	1528	1556	rBV	182054	354457	51.19%	5.955%
9	6.694	1650	1665	1687	rBV	147265	289171	41.76%	4.858%
10	6.797	1687	1697	1707	rVB6	4605	8488	1.23%	0.143%
11	7.568	1925	1937	1955	rBV2	82186	142545	20.59%	2.395%
12	7.900	2027	2040	2052	rBV	284726	524582	75.76%	8.813%
13	7.973	2052	2063	2094	rVB	304097	577457	83.40%	9.701%
14	8.182	2117	2128	2143	rBV	49762	82654	11.94%	1.389%
15	8.636	2256	2269	2285	rBV	406289	692419	100.00%	11.633%
16	9.420	2499	2513	2542	rBV	273783	474693	68.56%	7.975%
17	10.083	2710	2719	2733	rBV	13858	23470	3.39%	0.394%
18	10.758	2918	2929	2945	rBV	114237	183676	26.53%	3.086%
19	11.813	3245	3257	3280	rVB	343183	531504	76.76%	8.929%
20	12.195	3363	3376	3395	rBV	306631	493821	71.32%	8.296%
21	12.886	3582	3591	3604	rBV4	11128	17398	2.51%	0.292%




Sum of corrected areas: 5952371

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021822\
Data File : VU047214.D
Acq On : 17 Feb 2022 19:10
Operator : SY/MD
Sample : N1559-11DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M85DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

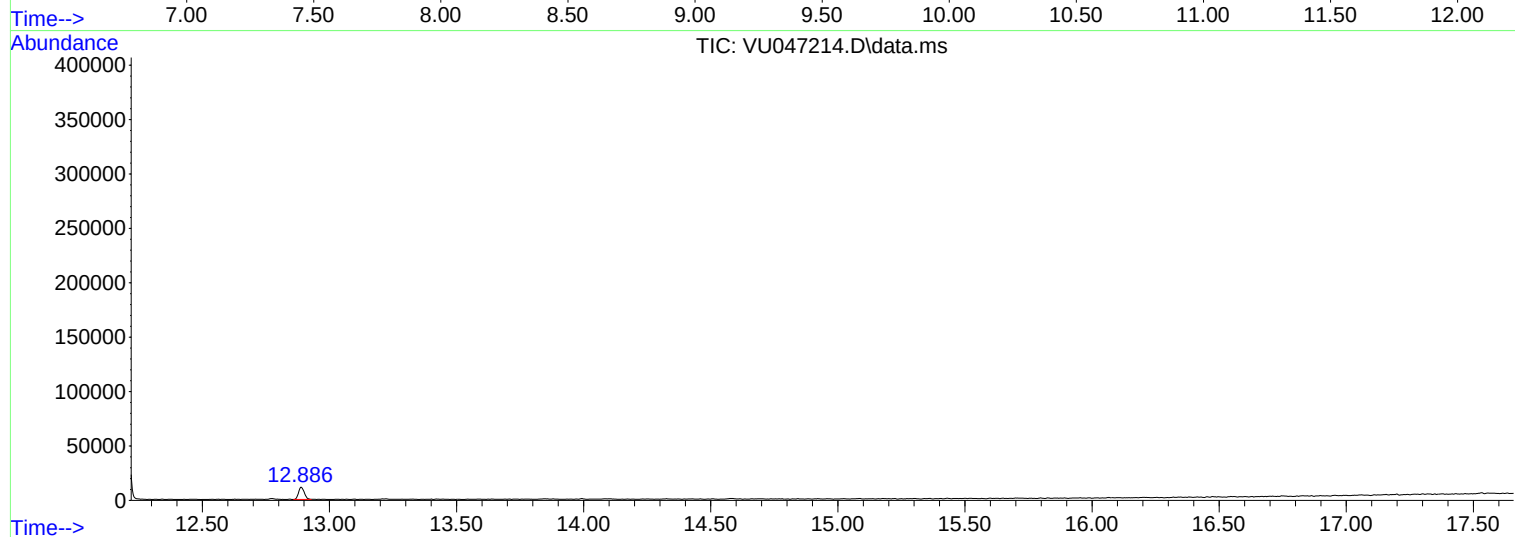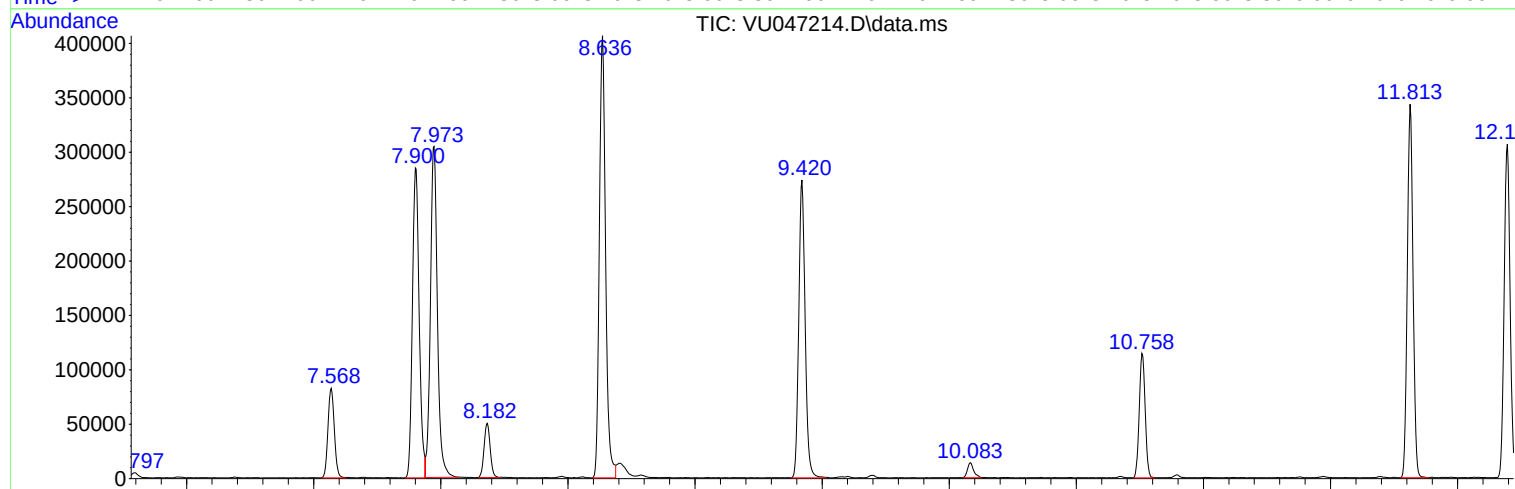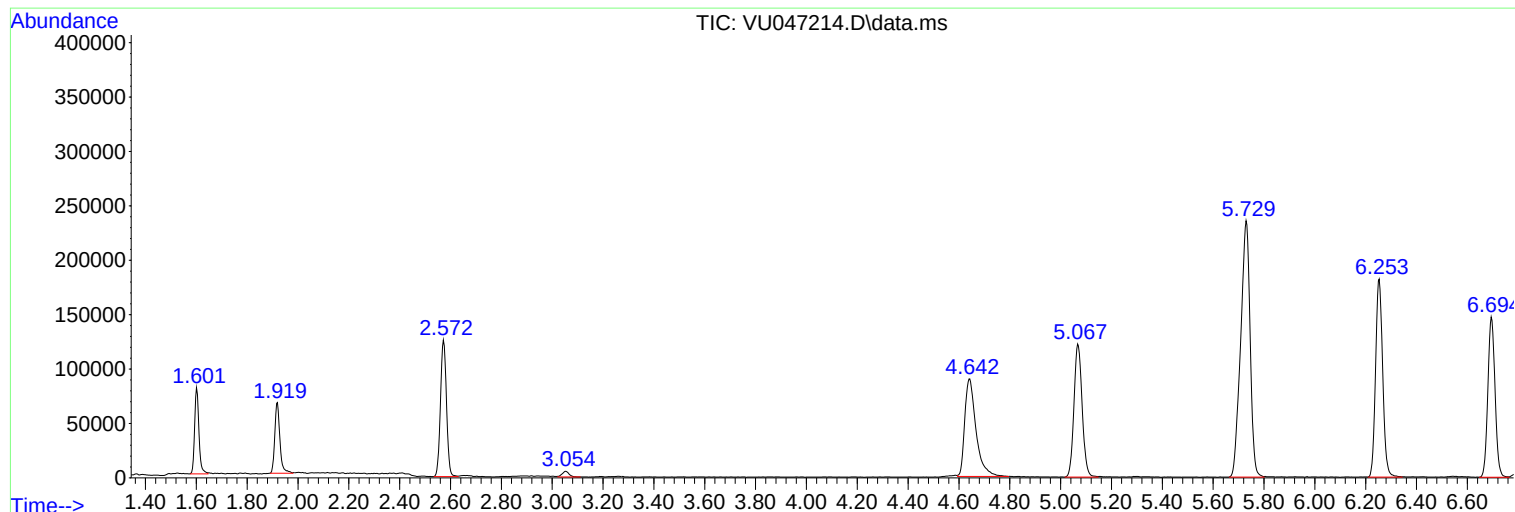

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021822\
Data File : VU047214.D
Acq On : 17 Feb 2022 19:10
Operator : SY/MD
Sample : N1559-11DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M85DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021822\
Data File : VU047214.D
Acq On : 17 Feb 2022 19:10
Operator : SY/MD
Sample : N1559-11DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M85DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc