


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021822\
Data File : VU047204.D
Acq On : 17 Feb 2022 14:33
Operator : SY/MD
Sample : BFB057
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB057

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Feb 18 03:32:37 2022

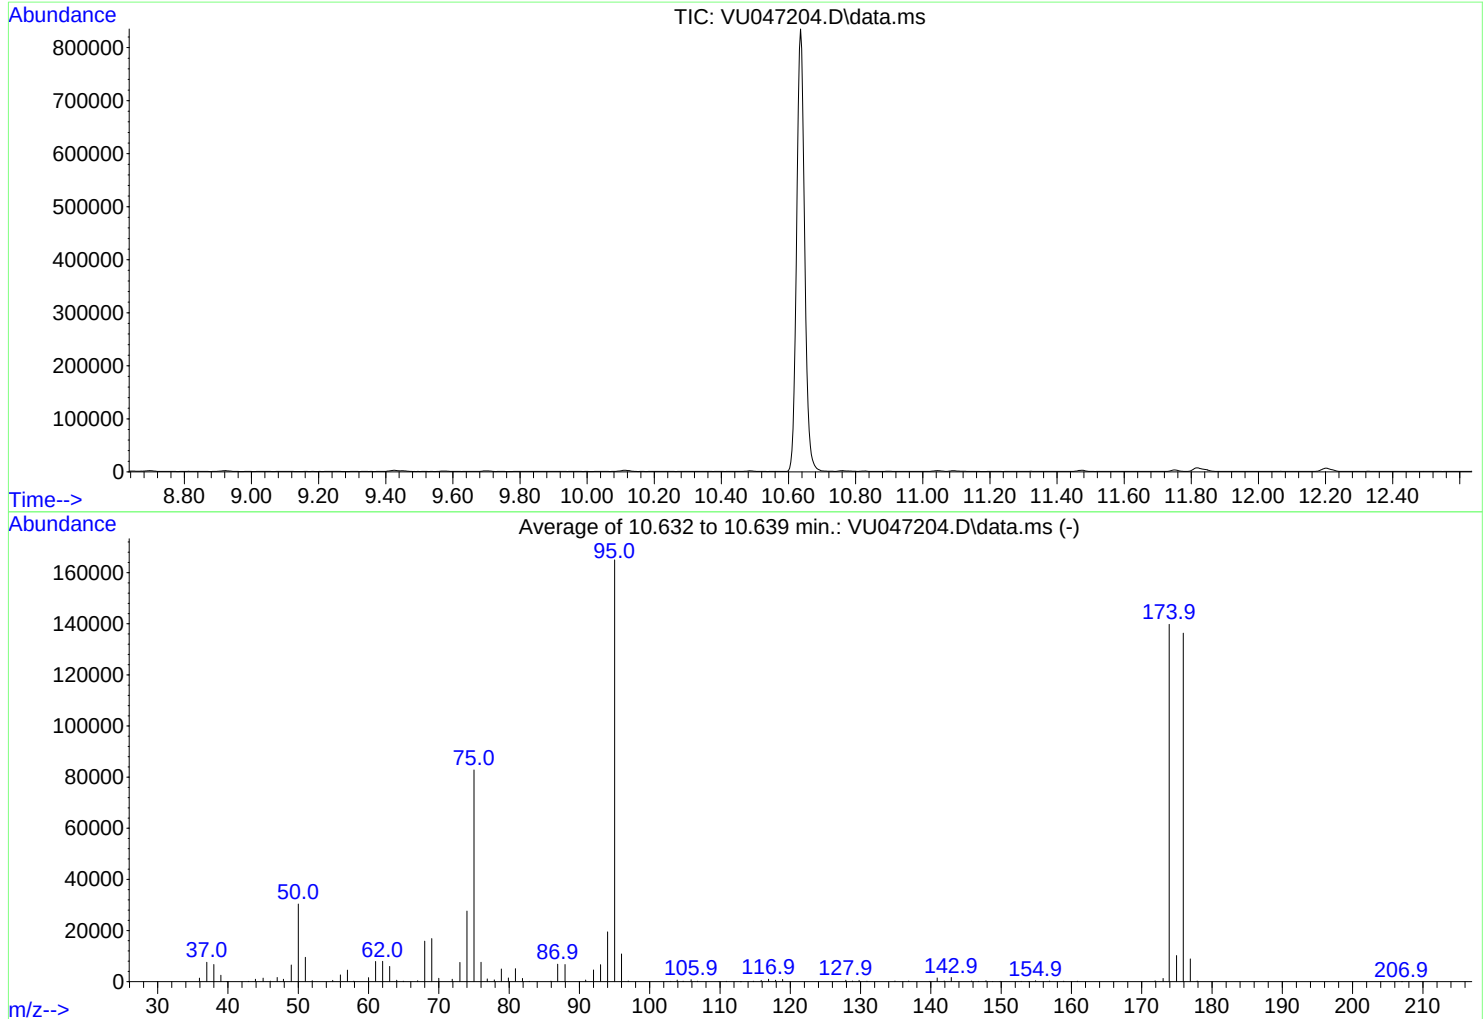

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	30376	PASS
75	95	30	80	50.2	82800	PASS
95	95	100	100	100.0	165013	PASS
96	95	5	9	6.5	10800	PASS
173	174	0.00	2	0.9	1265	PASS
174	95	50	120	84.7	139797	PASS
175	174	5	9	7.3	10212	PASS
176	174	95	101	97.5	136355	PASS
177	176	5	9	6.5	8895	PASS

Scan 2876 (10.587 min): VU047204.D\data.ms
BFB057

m/z	Abundance
39.80	163.0
43.90	475.0
206.90	253.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057

m/z	Abundance
36.00	1388.0
37.00	7608.0
38.00	6664.0
39.00	2543.0
39.90	216.0
42.90	135.0
44.00	1338.0
45.00	1479.0
46.00	168.0
47.00	1649.0
47.90	902.0
49.00	6654.0
50.00	30552.0
51.00	9473.0
52.00	440.0
54.90	492.0
56.00	2595.0
57.00	4702.0
57.90	203.0
60.00	1581.0
61.00	7855.0
62.00	8027.0
63.00	5894.0
64.00	570.0
64.90	175.0
67.00	368.0
68.00	16010.0
69.00	16872.0
70.00	1373.0
71.90	980.0
73.00	7558.0
74.00	27120.0
75.00	82264.0
76.00	7663.0
76.90	1072.0
77.90	635.0
78.90	4930.0
79.90	1450.0
80.90	4920.0
81.90	1250.0
82.90	101.0
85.90	225.0
86.90	6862.0
87.90	6397.0
90.90	601.0
92.00	4618.0
93.00	6763.0
94.00	19152.0
95.00	162944.0
96.00	11025.0
97.00	293.0
103.00	114.0
103.90	625.0
104.80	213.0
105.90	764.0
106.80	174.0
110.90	112.0
112.90	100.0
114.80	156.0
115.90	521.0
116.90	894.0
117.90	540.0
118.90	850.0
127.90	530.0
128.90	288.0
129.80	516.0
130.90	178.0
134.90	263.0
136.90	250.0
139.80	131.0
140.90	1490.0
141.90	233.0
142.90	1611.0
145.80	223.0
146.80	129.0
147.80	355.0
149.90	150.0
152.80	135.0
153.90	113.0
154.90	385.0
156.90	231.0
158.90	175.0
160.90	183.0
171.90	314.0
173.00	1171.0
173.90	135360.0
175.00	10013.0
175.90	131048.0
176.90	8681.0
177.90	241.0
207.00	230.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057

m/z	Abundance
36.00	1428.0
37.00	7835.0
38.00	6944.0
39.00	2630.0
39.90	192.0
42.90	143.0
44.00	1483.0
45.00	1451.0
46.00	181.0
47.00	1720.0
47.90	965.0
49.00	6665.0
50.00	31264.0
51.00	9831.0
52.00	425.0
54.90	490.0
56.00	2739.0
57.00	4623.0
57.90	189.0
60.00	1624.0
61.00	8132.0
62.00	8221.0
63.00	6161.0
64.00	556.0
64.90	172.0
67.00	421.0
68.00	16338.0
69.00	17488.0
70.00	1364.0
71.90	953.0
73.00	7784.0
74.00	28544.0
75.00	85224.0
76.00	7835.0
76.90	1081.0
77.90	700.0
78.90	5115.0
79.90	1525.0
80.90	5208.0
81.90	1322.0
82.80	134.0
85.90	203.0
86.90	7032.0
87.90	6904.0
90.90	621.0
92.00	4730.0
93.00	6838.0
94.00	20120.0
95.00	169856.0
96.00	11040.0
97.00	264.0
103.00	117.0
103.90	672.0
104.80	209.0
105.90	799.0
106.80	166.0
109.90	116.0
110.90	113.0
114.70	166.0
115.90	517.0
116.90	953.0
117.90	557.0
118.90	929.0
127.90	578.0
128.90	290.0
129.80	514.0
130.90	190.0
134.90	286.0
136.90	301.0
139.90	147.0
140.90	1513.0
141.90	234.0
142.90	1698.0
145.80	243.0
146.80	122.0
147.90	404.0
148.80	100.0
149.80	156.0
152.80	129.0
153.80	104.0
154.90	404.0
156.90	269.0
158.90	194.0
160.80	171.0
171.90	334.0
173.10	1305.0
173.90	144256.0
175.00	10512.0
175.90	140736.0
176.90	9220.0
177.90	237.0
207.00	273.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057

m/z	Abundance
35.90	1326.0
37.00	7253.0
38.00	6565.0
39.00	2424.0
39.90	182.0
42.90	125.0
43.90	1487.0
45.00	1301.0
46.10	173.0
47.00	1548.0
47.90	910.0
49.00	6221.0
50.00	29312.0
51.00	9312.0
52.00	361.0
54.90	460.0
56.00	2603.0
57.00	4286.0
57.90	168.0
60.00	1459.0
61.00	7626.0
62.00	7563.0
63.00	5880.0
64.00	496.0
65.00	141.0
67.00	445.0
68.00	15219.0
69.00	16254.0
70.00	1229.0
71.90	840.0
73.00	7224.0
74.00	27120.0
75.00	80912.0
76.00	7227.0
76.90	1002.0
77.90	670.0
78.90	4827.0
79.90	1445.0
80.90	5046.0
81.90	1278.0
82.80	141.0
86.00	185.0
86.90	6666.0
88.00	6821.0
90.90	616.0
92.00	4456.0
93.00	6293.0
94.00	19144.0
95.00	162240.0
96.00	10334.0
96.90	250.0
103.00	100.0
103.90	668.0
104.70	189.0
105.90	694.0
106.80	148.0
109.80	124.0
110.90	102.0
114.70	165.0
115.80	514.0
116.90	925.0
117.90	539.0
118.90	905.0
127.90	579.0
128.80	245.0
129.80	517.0
130.90	202.0
134.90	265.0
136.80	306.0
139.90	128.0
140.90	1424.0
141.90	204.0
142.90	1616.0
145.80	248.0
146.80	103.0
147.90	418.0
148.80	128.0
149.80	149.0
152.90	101.0
154.90	401.0
156.90	275.0
158.90	191.0
160.90	139.0
171.90	310.0
173.10	1320.0
173.90	139776.0
174.90	10111.0
175.90	137280.0
176.90	8784.0
177.90	225.0
207.00	292.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057