

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU021919\
 Data File : VU029549.D
 Acq On : 19 Feb 2019 12:53
 Operator : JC/SP
 Sample : K1522-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM2

Quant Time: Feb 26 00:37:55 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Feb 20 00:07:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	211535	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	204893	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	106546	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	58735	4.13	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.60%
7) Chloroethane-d5	1.68	69	54856	4.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.40%
11) 1,1-Dichloroethene-d2	2.27	63	92230	2.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.60%#
20) 2-Butanone-d5	4.19	46	151478	51.26	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.52%
24) Chloroform-d	4.65	84	99732	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.20%
26) 1,2-Dichloroethane-d4	5.31	65	59355	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.60%
32) Benzene-d6	5.34	84	226949	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.20%
36) 1,2-Dichloropropane-d6	6.33	67	70457	4.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.80%
41) Toluene-d8	7.56	98	216787	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.20%
43) trans-1,3-Dichloropropene-	7.85	79	26962	4.15	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.00%
46) 2-Hexanone-d5	8.31	63	145618	48.63	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.26%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	60732	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.00%
64) 1,2-Dichlorobenzene-d4	11.86	152	98192	5.00	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.00%


Target Compounds					Ovalue
13) Acetone	2.32	43	5698	2.123 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU021919\
Data File : VU029549.D
Acq On : 19 Feb 2019 12:53
Operator : JC/SP
Sample : K1522-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM2

Quant Time: Feb 26 00:37:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Feb 20 00:07:58 2019
Response via : Initial Calibration

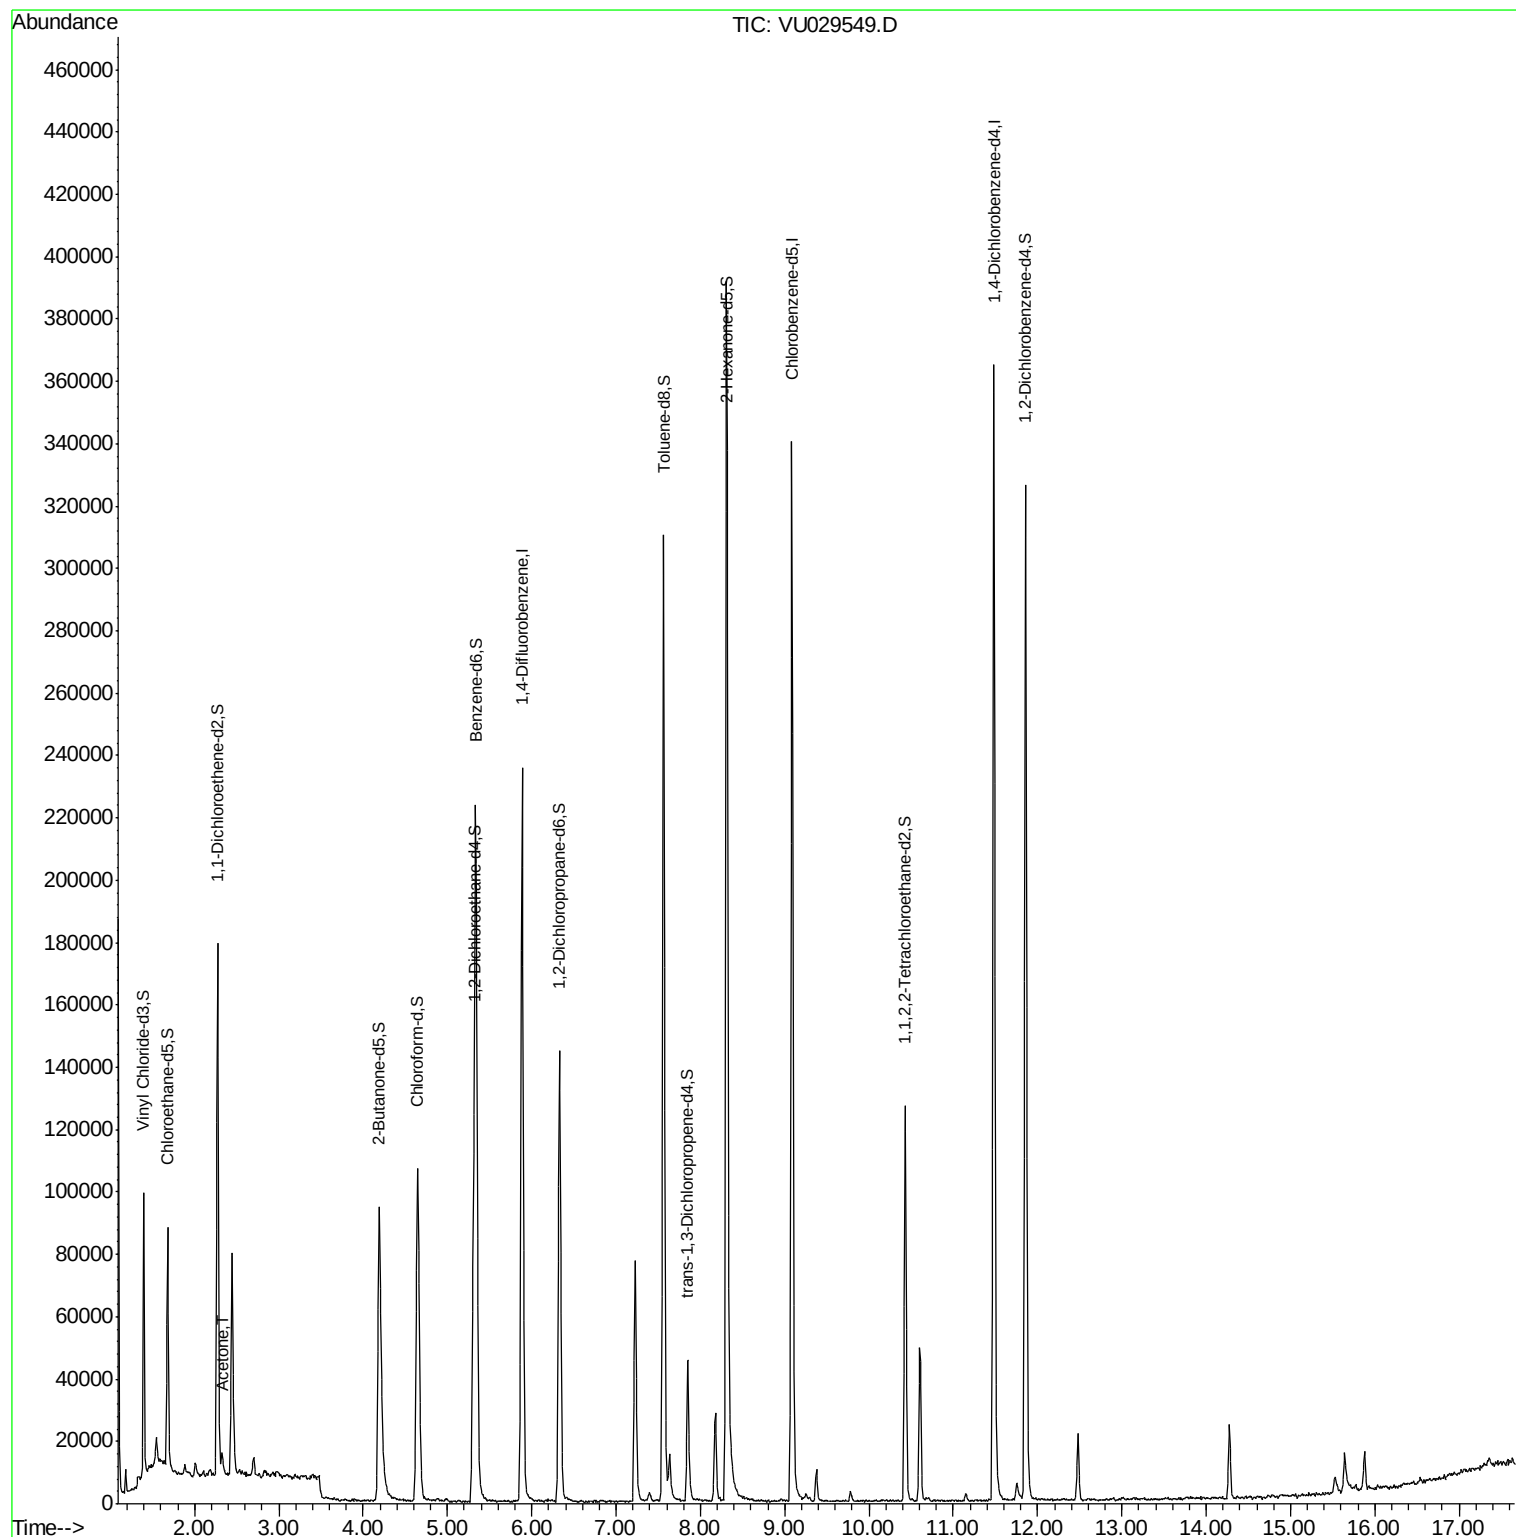

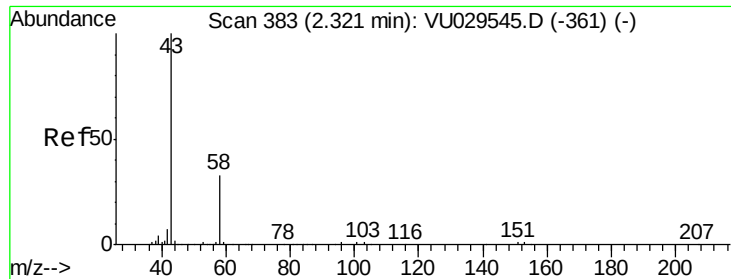

#13

Acetone

Concen: 2.123 ug/L

RT: 2.32 min Scan# 384

Delta R.T. 0.00 min

Lab File: VU029549.D

Acq: 19 Feb 2019 12:53

Instrument :
MSVOA_U
ClientSampleId :
C0AM2

Tot Ion: 43 Resp: 5698

Ion Ratio Lower Upper

43 100

58 40.2 0.0 65.0

