


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU021919\
 Data File : VU029544.D
 Acq On : 19 Feb 2019 10:35
 Operator : JC/SP
 Sample : BFB40
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB40

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Feb 21 04:23:07 2019

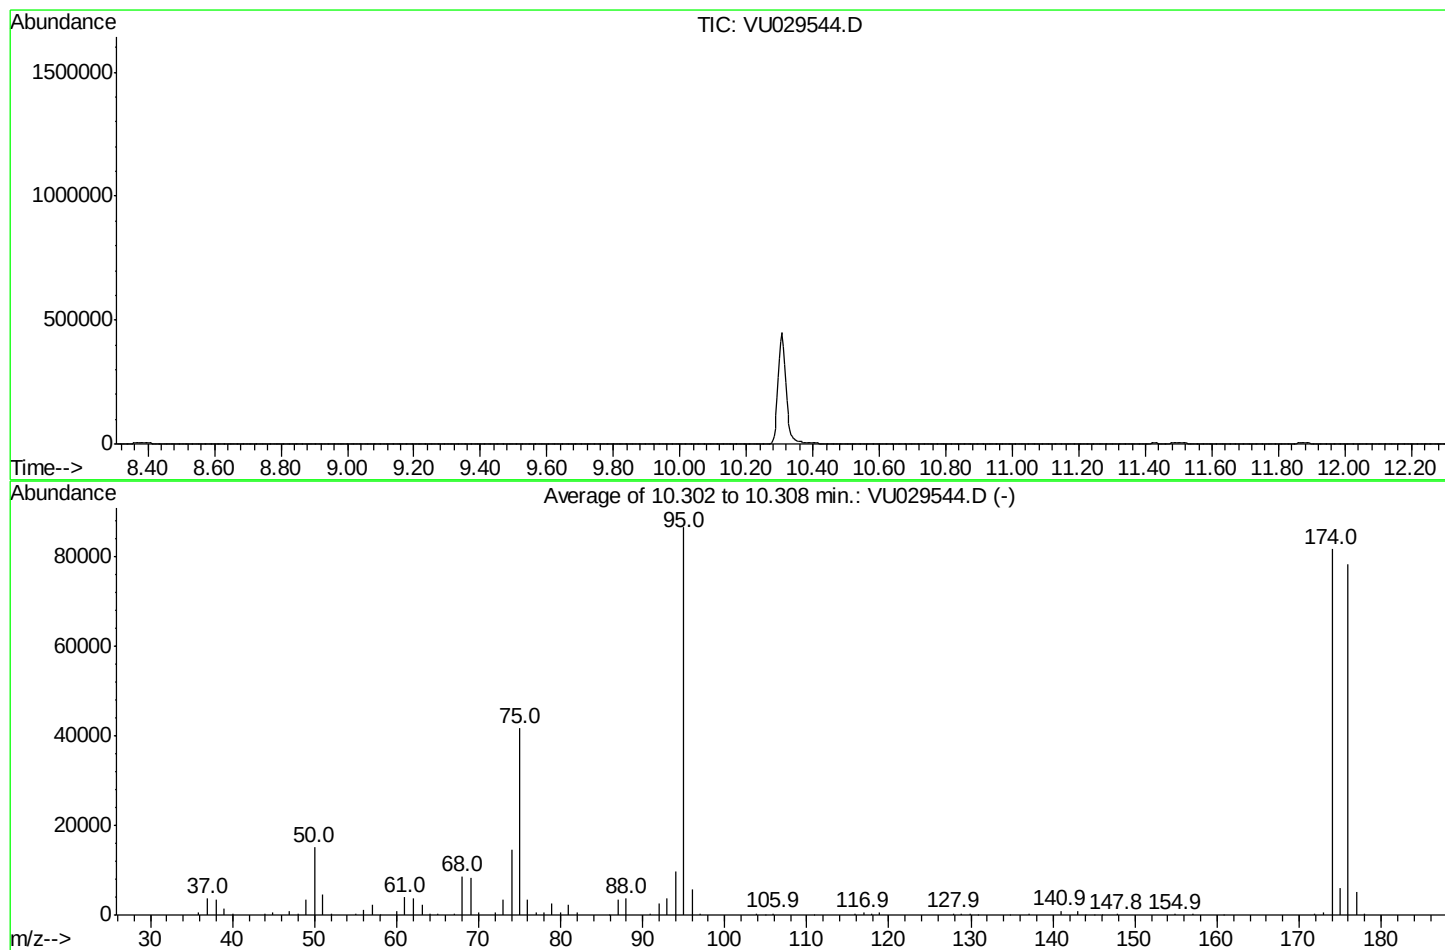

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	15061	PASS
75	95	30	80	48.1	41645	PASS
95	95	100	100	100.0	86541	PASS
96	95	5	9	6.6	5725	PASS
173	174	0.00	2	0.8	688	PASS
174	95	50	120	94.3	81640	PASS
175	174	5	9	7.5	6137	PASS
176	174	95	101	96.1	78440	PASS
177	176	5	9	6.5	5119	PASS

Scan 2852 (10.260 min): VU029544.D
BFB40

m/z	Abundance
41.10	104.0
42.90	128.0
43.90	692.0
207.00	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
35.90	661.0
37.00	3670.0
38.00	3303.0
39.00	1345.0
40.00	153.0
44.00	1070.0
44.90	607.0
47.00	842.0
48.00	457.0
49.00	3285.0
50.00	14722.0
51.00	4629.0
52.00	235.0
55.00	332.0
56.00	1314.0
57.00	2274.0
58.00	100.0
60.00	955.0
61.00	3690.0
62.00	3620.0
63.10	2135.0
64.00	213.0
64.90	195.0
67.00	229.0
68.00	8209.0
69.00	8379.0
70.00	594.0
72.00	450.0
73.00	3193.0
74.00	14001.0
75.00	39816.0
76.00	3156.0
77.00	514.0
77.90	488.0
78.90	2399.0
79.90	732.0
80.90	2304.0
82.00	648.0
85.90	108.0
87.00	3513.0
88.00	3320.0
90.90	296.0
92.00	2500.0
93.00	3633.0
94.00	9612.0
95.00	82512.0
96.00	5584.0
96.90	187.0
103.80	303.0
104.90	116.0
105.90	350.0
115.90	221.0
116.90	508.0
117.80	299.0
118.80	425.0
127.90	327.0
128.80	196.0
129.80	280.0
130.90	134.0
137.10	161.0
140.90	820.0
143.00	910.0
145.00	123.0
145.90	123.0
147.80	166.0
154.80	205.0
157.10	176.0
172.00	340.0
172.90	690.0
174.00	76640.0
175.00	5767.0
176.00	74040.0
177.00	4875.0
178.00	192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
35.90	640.0
37.00	3843.0
38.00	3565.0
39.00	1423.0
40.00	155.0
42.90	108.0
43.90	1004.0
44.90	665.0
46.90	809.0
47.90	421.0
49.00	3421.0
50.00	15636.0
51.00	4794.0
52.00	298.0
55.00	317.0
56.00	1297.0
57.00	2312.0
57.90	107.0
60.00	1019.0
61.00	4123.0
62.00	3782.0
63.10	2525.0
64.00	235.0
64.90	182.0
67.00	285.0
68.00	8751.0
69.00	8669.0
70.10	607.0
72.00	488.0
73.00	3364.0
74.00	15130.0
75.00	42984.0
76.00	3441.0
77.00	535.0
77.90	461.0
78.90	2528.0
79.90	725.0
80.90	2354.0
81.90	742.0
87.00	3360.0
87.90	3804.0
90.90	327.0
92.00	2621.0
93.00	3740.0
94.00	9957.0
95.00	89360.0
96.00	5847.0
96.90	224.0
103.90	353.0
104.90	112.0
105.90	416.0
115.90	239.0
116.90	567.0
117.80	297.0
118.80	478.0
127.90	361.0
128.90	185.0
129.90	315.0
130.90	143.0
134.80	117.0
137.00	220.0
141.00	908.0
142.90	911.0
144.00	106.0
145.90	160.0
147.80	178.0
154.90	198.0
157.00	179.0
160.80	106.0
172.00	368.0
172.90	710.0
174.00	84336.0
175.00	6340.0
176.00	81056.0
177.00	5271.0
177.90	158.0
206.90	146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
35.90	560.0
37.00	3590.0
38.00	3433.0
39.00	1235.0
40.00	172.0
43.90	934.0
44.90	634.0
47.00	724.0
47.90	383.0
49.00	3233.0
50.00	14827.0
51.00	4670.0
52.00	303.0
55.10	280.0
56.00	1208.0
57.00	2249.0
58.00	102.0
60.00	937.0
61.00	4037.0
62.00	3625.0
63.10	2601.0
64.00	265.0
65.00	130.0
67.00	305.0
68.00	8450.0
69.00	8144.0
70.10	599.0
72.10	514.0
73.00	3357.0
74.00	14680.0
75.00	42136.0
76.00	3378.0
77.00	558.0
77.90	376.0
78.90	2469.0
80.00	648.0
81.00	2404.0
81.90	732.0
85.90	115.0
87.00	3145.0
87.90	3716.0
90.90	301.0
92.00	2546.0
93.00	3479.0
94.00	9822.0
95.00	87752.0
96.00	5744.0
97.00	202.0
103.90	412.0
105.90	436.0
110.90	126.0
115.80	270.0
116.90	552.0
117.90	294.0
118.80	454.0
127.90	316.0
128.80	166.0
129.90	368.0
130.80	147.0
134.80	169.0
137.00	204.0
141.00	958.0
142.90	851.0
145.90	157.0
147.80	202.0
155.00	217.0
156.90	189.0
160.80	129.0
171.90	327.0
173.00	664.0
174.00	83944.0
175.00	6306.0
176.00	80224.0
177.00	5211.0
177.90	111.0
207.00	176.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40