
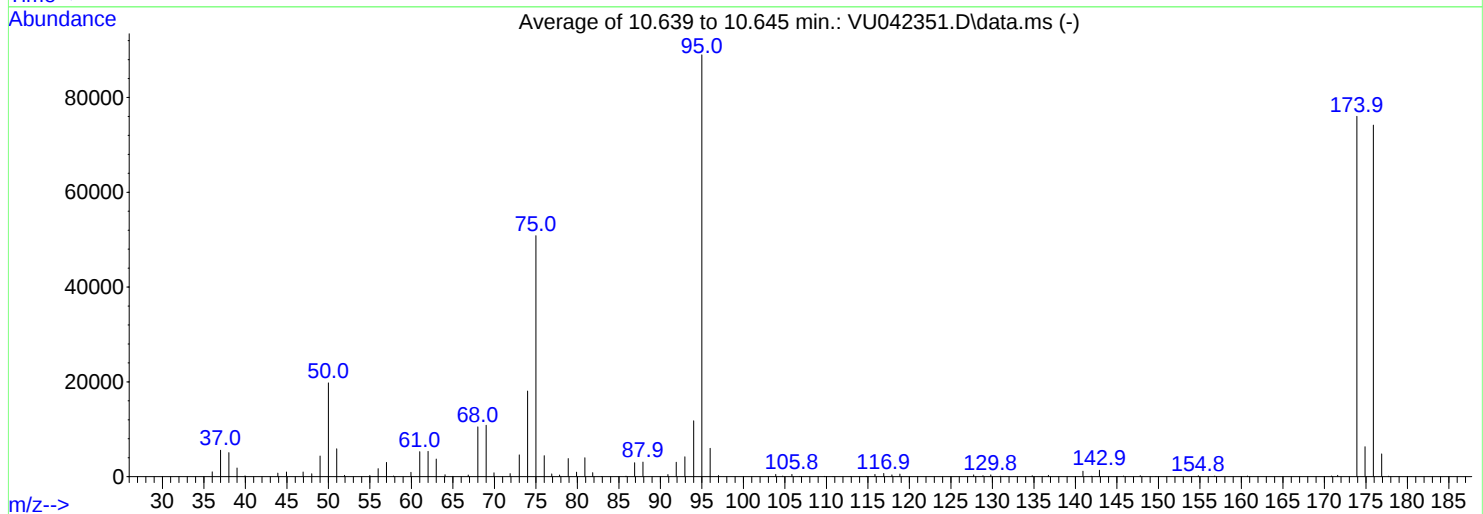


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021921\
Data File : VU042351.D
Acq On : 19 Feb 2021 09:21
Operator : SY/MD
Sample : BFB46
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB46

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR021921WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Feb 19 13:39:55 2021

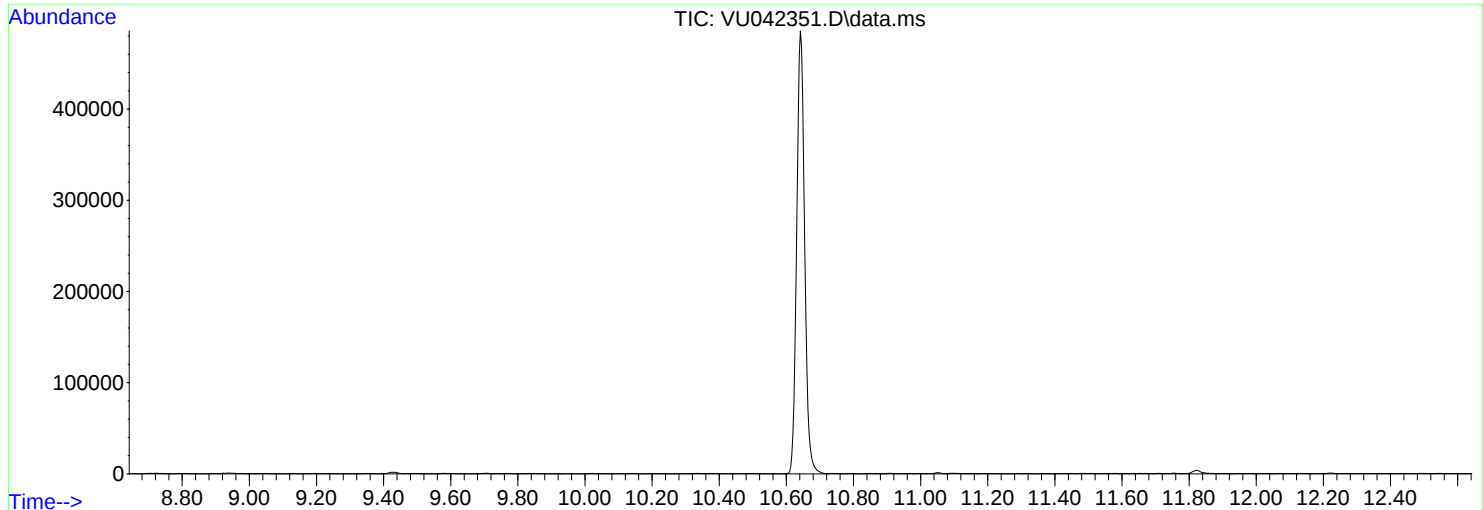

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.2	19784	PASS
75	95	30	80	57.1	50837	PASS
95	95	100	100	100.0	89005	PASS
96	95	5	9	6.7	5974	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.4	76021	PASS
175	174	5	9	8.3	6308	PASS
176	174	95	101	97.6	74181	PASS
177	176	5	9	6.5	4807	PASS

m/z	Abundance
36.00	1002.0
37.00	5386.0
38.00	4933.0
39.00	1904.0
39.90	177.0
43.90	918.0
45.00	963.0
47.00	1107.0
48.00	674.0
49.00	4201.0
50.00	20000.0
51.00	5826.0
51.90	278.0
55.00	195.0
56.00	1656.0
57.00	2874.0
57.80	150.0
60.00	942.0
61.00	5135.0
62.00	5150.0
63.00	3813.0
64.00	413.0
65.00	139.0
66.80	330.0
68.00	10391.0
69.00	10659.0
69.90	773.0
71.90	618.0
73.00	4496.0
74.00	17736.0
75.00	50376.0
76.00	4287.0
76.90	589.0
77.90	388.0
78.90	3868.0
79.90	947.0
80.90	3906.0
81.90	919.0
85.90	104.0
86.90	2953.0
87.90	3024.0
90.90	412.0
91.90	2935.0
92.90	4219.0
94.00	11285.0
95.00	86928.0
96.00	5938.0
97.00	254.0
103.90	442.0
104.70	133.0
105.90	512.0
109.80	128.0
110.80	100.0
112.90	112.0
114.80	133.0
115.90	432.0
116.90	645.0
117.90	370.0
118.90	535.0
127.80	330.0
128.90	186.0
129.80	334.0
131.00	131.0
134.80	234.0
136.70	248.0
140.90	1166.0
142.90	1234.0
145.80	125.0
147.80	204.0
154.80	190.0
156.80	169.0
160.70	118.0
170.80	134.0
171.60	250.0
173.90	72784.0
174.90	6228.0
175.90	69592.0
176.90	4582.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	1068.0
37.00	5776.0
38.00	5183.0
39.00	1805.0
39.90	161.0
43.90	946.0
44.90	1005.0
46.90	983.0
48.00	615.0
49.00	4458.0
50.00	20336.0
51.00	6061.0
52.00	262.0
55.00	240.0
56.00	1759.0
57.00	3100.0
57.80	153.0
60.00	950.0
61.00	5385.0
62.00	5515.0
63.00	3822.0
64.10	392.0
65.00	119.0
66.90	333.0
68.00	10834.0
69.00	11206.0
70.00	845.0
71.90	682.0
73.00	4720.0
74.00	18616.0
75.00	52512.0
76.00	4567.0
76.90	588.0
77.90	361.0
78.90	3947.0
79.90	959.0
80.90	4101.0
81.80	849.0
82.90	101.0
85.80	118.0
86.90	2956.0
87.90	3125.0
90.90	457.0
91.90	3134.0
93.00	4376.0
94.00	12158.0
95.00	91808.0
96.00	6129.0
97.00	253.0
103.90	473.0
104.70	127.0
105.80	487.0
106.80	127.0
109.80	110.0
114.80	108.0
115.80	494.0
116.90	685.0
117.90	391.0
118.80	588.0
127.80	364.0
128.80	209.0
129.80	398.0
131.00	115.0
134.80	205.0
136.80	279.0
140.90	1191.0
141.90	131.0
142.90	1413.0
145.80	132.0
147.80	214.0
154.80	190.0
156.80	142.0
160.80	138.0
170.90	155.0
171.60	280.0
173.90	78296.0
174.90	6531.0
175.90	76656.0
176.90	4954.0
177.80	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	988.0
37.00	5581.0
38.00	5090.0
39.00	1773.0
40.00	149.0
43.90	906.0
45.00	968.0
46.90	863.0
48.00	506.0
49.00	4393.0
50.00	19016.0
51.00	5752.0
52.00	232.0
55.00	299.0
56.00	1687.0
57.00	3061.0
57.90	132.0
59.90	868.0
61.00	5332.0
62.00	5296.0
63.00	3508.0
64.00	381.0
66.90	322.0
68.00	10328.0
69.00	10621.0
70.00	788.0
71.90	642.0
73.00	4520.0
74.00	17880.0
75.00	49624.0
76.00	4383.0
76.90	559.0
77.80	288.0
78.90	3670.0
79.90	935.0
80.90	3919.0
81.90	756.0
85.80	112.0
86.90	2949.0
87.90	3033.0
90.90	432.0
91.90	3033.0
93.00	3997.0
94.00	11967.0
95.00	88280.0
96.00	5855.0
97.00	196.0
103.90	482.0
104.80	118.0
105.80	460.0
106.80	128.0
115.80	454.0
116.90	691.0
117.90	384.0
118.80	552.0
127.70	373.0
128.80	202.0
129.80	429.0
130.90	105.0
134.80	162.0
136.80	257.0
140.90	1090.0
141.90	146.0
142.90	1370.0
145.80	135.0
147.80	227.0
149.70	128.0
154.80	194.0
156.80	125.0
160.80	112.0
170.90	140.0
171.60	261.0
173.90	76984.0
174.90	6166.0
175.90	76296.0
176.90	4885.0
177.70	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
43.90	172.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46