


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU022019\
 Data File : VU029570.D
 Acq On : 20 Feb 2019 07:58
 Operator : JC/SP
 Sample : BFB46
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB46

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Feb 21 04:23:07 2019

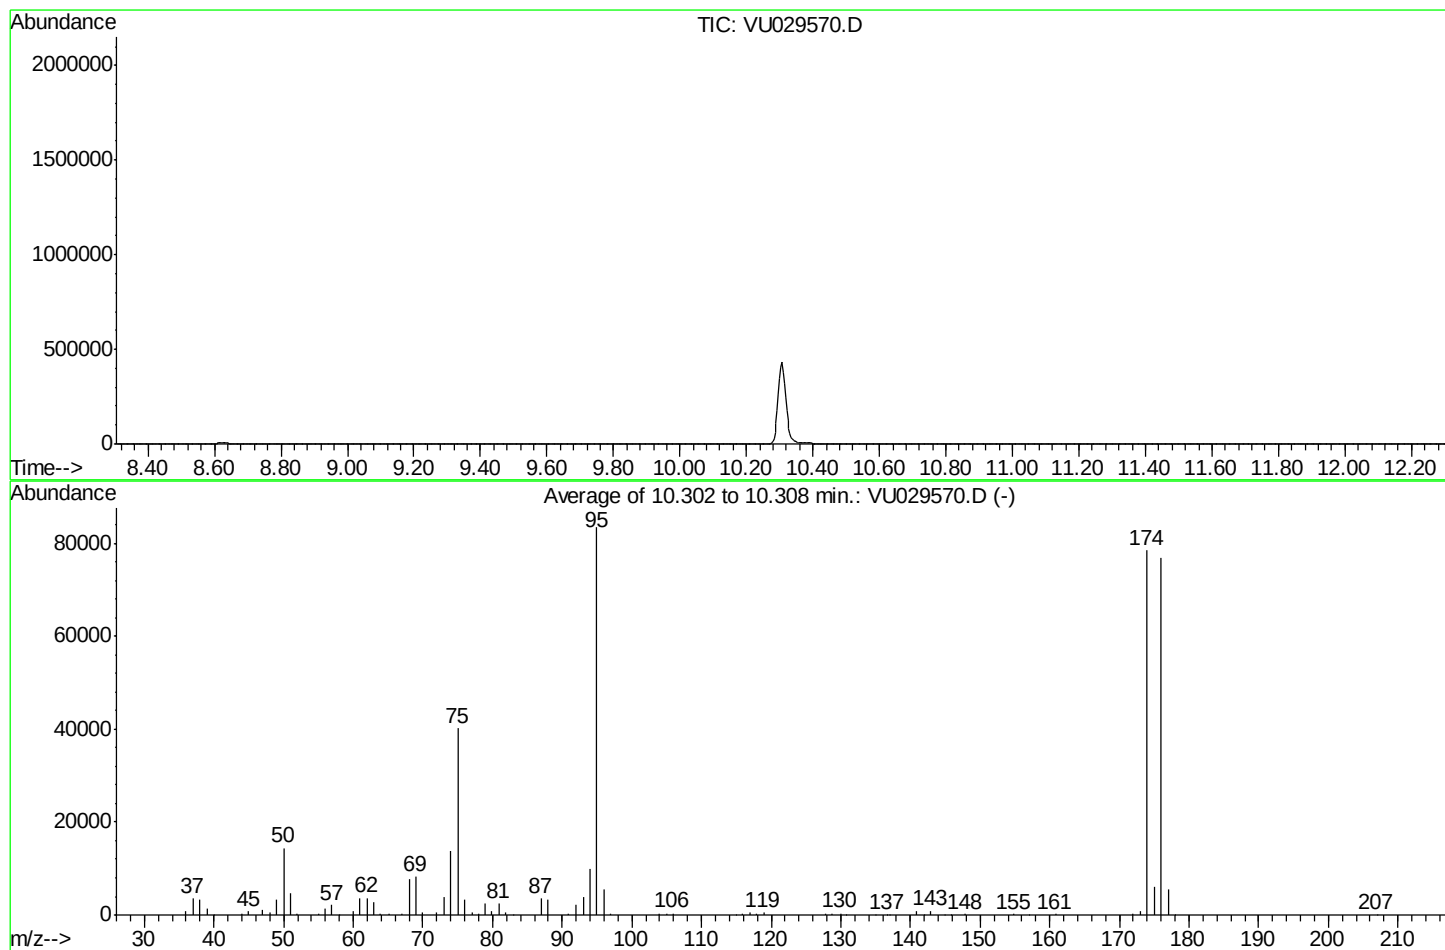

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	14406	PASS
75	95	30	80	48.2	40226	PASS
95	95	100	100	100.0	83440	PASS
96	95	5	9	6.6	5483	PASS
173	174	0.00	2	1.0	763	PASS
174	95	50	120	94.0	78413	PASS
175	174	5	9	7.7	6033	PASS
176	174	95	101	98.0	76872	PASS
177	176	5	9	7.1	5449	PASS

m/z	Abundance
39.90	121.0
43.90	520.0
207.00	148.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	620.0
37.00	3413.0
38.00	3067.0
39.00	1355.0
40.00	146.0
44.00	926.0
45.00	692.0
47.00	1068.0
48.00	470.0
49.00	3150.0
50.00	13991.0
51.00	4454.0
52.00	360.0
55.00	212.0
56.00	1307.0
56.90	2124.0
60.00	731.0
61.00	3461.0
62.00	3799.0
63.00	2751.0
63.90	266.0
65.10	226.0
67.00	134.0
68.00	7909.0
69.00	8103.0
70.00	646.0
72.00	552.0
73.00	3849.0
74.00	13934.0
75.00	39584.0
76.00	3348.0
77.00	542.0
77.90	380.0
78.90	2562.0
79.90	820.0
80.90	2280.0
81.90	573.0
87.00	3650.0
88.00	3123.0
90.90	289.0
92.00	2333.0
93.00	3610.0
94.00	9747.0
95.00	83768.0
96.00	5490.0
96.90	208.0
104.00	383.0
105.00	162.0
105.90	320.0
115.80	218.0
116.80	424.0
117.80	274.0
118.90	498.0
127.90	314.0
128.80	134.0
129.90	388.0
130.80	114.0
134.90	104.0
140.90	815.0
141.90	110.0
142.90	1045.0
145.00	121.0
145.80	153.0
147.80	176.0
154.90	253.0
157.00	125.0
160.80	206.0
172.00	397.0
172.90	747.0
174.00	80216.0
175.00	5968.0
176.00	78584.0
177.00	5531.0
206.90	153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	779.0
37.00	3645.0
38.00	3345.0
39.00	1423.0
39.90	144.0
44.00	907.0
45.00	764.0
47.00	1025.0
48.00	560.0
49.00	3320.0
50.00	14792.0
51.00	4798.0
52.00	341.0
55.00	238.0
56.00	1307.0
56.90	2108.0
58.00	136.0
60.00	759.0
61.00	3630.0
62.00	3824.0
63.00	2849.0
63.90	296.0
65.10	261.0
67.00	140.0
68.00	7951.0
69.00	8413.0
70.00	654.0
72.00	532.0
73.00	4077.0
74.00	14164.0
75.00	41336.0
76.00	3426.0
77.00	515.0
77.90	423.0
78.90	2689.0
79.90	814.0
80.90	2490.0
81.90	599.0
82.90	121.0
87.00	3616.0
88.00	3278.0
90.80	338.0
92.00	2300.0
93.00	3857.0
94.00	10261.0
95.00	85872.0
96.00	5610.0
96.90	210.0
104.00	302.0
104.90	188.0
105.90	350.0
114.90	118.0
115.80	293.0
116.90	493.0
117.80	263.0
118.90	535.0
127.90	294.0
128.80	164.0
130.00	365.0
130.80	107.0
136.70	106.0
140.90	871.0
142.90	955.0
145.00	115.0
145.80	128.0
147.90	152.0
154.90	267.0
157.00	123.0
160.80	199.0
172.00	394.0
172.90	798.0
174.00	80432.0
175.00	6223.0
176.00	79224.0
177.00	5622.0
177.90	109.0
207.00	186.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	834.0
37.00	3509.0
38.00	3304.0
39.00	1456.0
40.00	138.0
44.00	840.0
45.00	717.0
47.00	869.0
48.00	547.0
49.00	3143.0
50.00	14436.0
51.00	4651.0
51.90	278.0
55.00	215.0
56.00	1254.0
57.00	2019.0
57.90	115.0
60.00	700.0
61.00	3520.0
62.00	3544.0
63.00	2682.0
63.90	327.0
65.00	251.0
66.90	196.0
68.00	7223.0
69.00	7915.0
70.00	619.0
72.00	411.0
73.00	3675.0
74.00	13066.0
75.00	39760.0
76.00	3315.0
77.10	531.0
78.00	416.0
78.90	2601.0
79.90	709.0
80.90	2638.0
81.90	624.0
82.90	112.0
87.00	3306.0
88.00	3218.0
90.80	355.0
92.00	2072.0
93.00	3843.0
94.00	9529.0
95.00	80680.0
96.00	5351.0
96.90	171.0
103.90	251.0
104.90	170.0
105.90	312.0
115.00	110.0
115.90	347.0
117.00	498.0
117.80	220.0
119.00	499.0
127.80	256.0
128.70	177.0
130.00	319.0
136.70	117.0
137.00	108.0
140.90	867.0
142.90	798.0
144.90	115.0
145.90	122.0
147.90	164.0
154.90	218.0
157.10	104.0
160.80	127.0
171.90	374.0
173.00	744.0
174.00	74592.0
175.00	5909.0
176.00	72808.0
177.00	5195.0
207.00	213.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46