

Data File : VU036869.D
Acq On : 20 Feb 2020 15:27
Operator : JC/MD
Sample : L1580-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBDW4

Quant Time: Feb 21 00:52:32 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Feb 21 00:49:14 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	141520	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	133619	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	52232	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	44374	3.65	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.00%
7) Chloroethane-d5	1.93	69	41803	3.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.20%
11) 1,1-Dichloroethene-d2	2.59	63	63519	3.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.40%
20) 2-Butanone-d5	4.67	46	121156	47.47	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.94%
24) Chloroform-d	5.11	84	79886	4.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.00%
26) 1,2-Dichloroethane-d4	5.74	65	46591	4.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.60%
32) Benzene-d6	5.76	84	176706	4.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.00%
36) 1,2-Dichloropropane-d6	6.73	67	57420	4.46	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.20%
41) Toluene-d8	7.93	98	159531	4.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.40%
43) trans-1,3-Dichloropropene-	8.20	79	19601	3.91	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.20%
46) 2-Hexanone-d5	8.66	63	100823	44.05	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.10%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	42699	4.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.00%
64) 1,2-Dichlorobenzene-d4	12.21	152	47794	4.58	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.60%

Target Compounds


					Qvalue
35) Methylcyclohexane	6.73	83	12517	0.751 ug/L #	19
37) 1,2-Dichloropropane	6.73	63	6137	0.545 ug/L #	89
39) cis-1,3-Dichloropropene	7.60	75	1442	0.089 ug/L #	53
59) 1,2,3-Trichloropropane	11.83	75	7938	1.068 ug/L	92
69) Naphthalene	14.12	128	24833	1.435 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU036869.D
Acq On : 20 Feb 2020 15:27
Operator : JC/MD
Sample : L1580-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBDW4

Quant Time: Feb 21 00:52:32 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Feb 21 00:49:14 2020
Response via : Initial Calibration

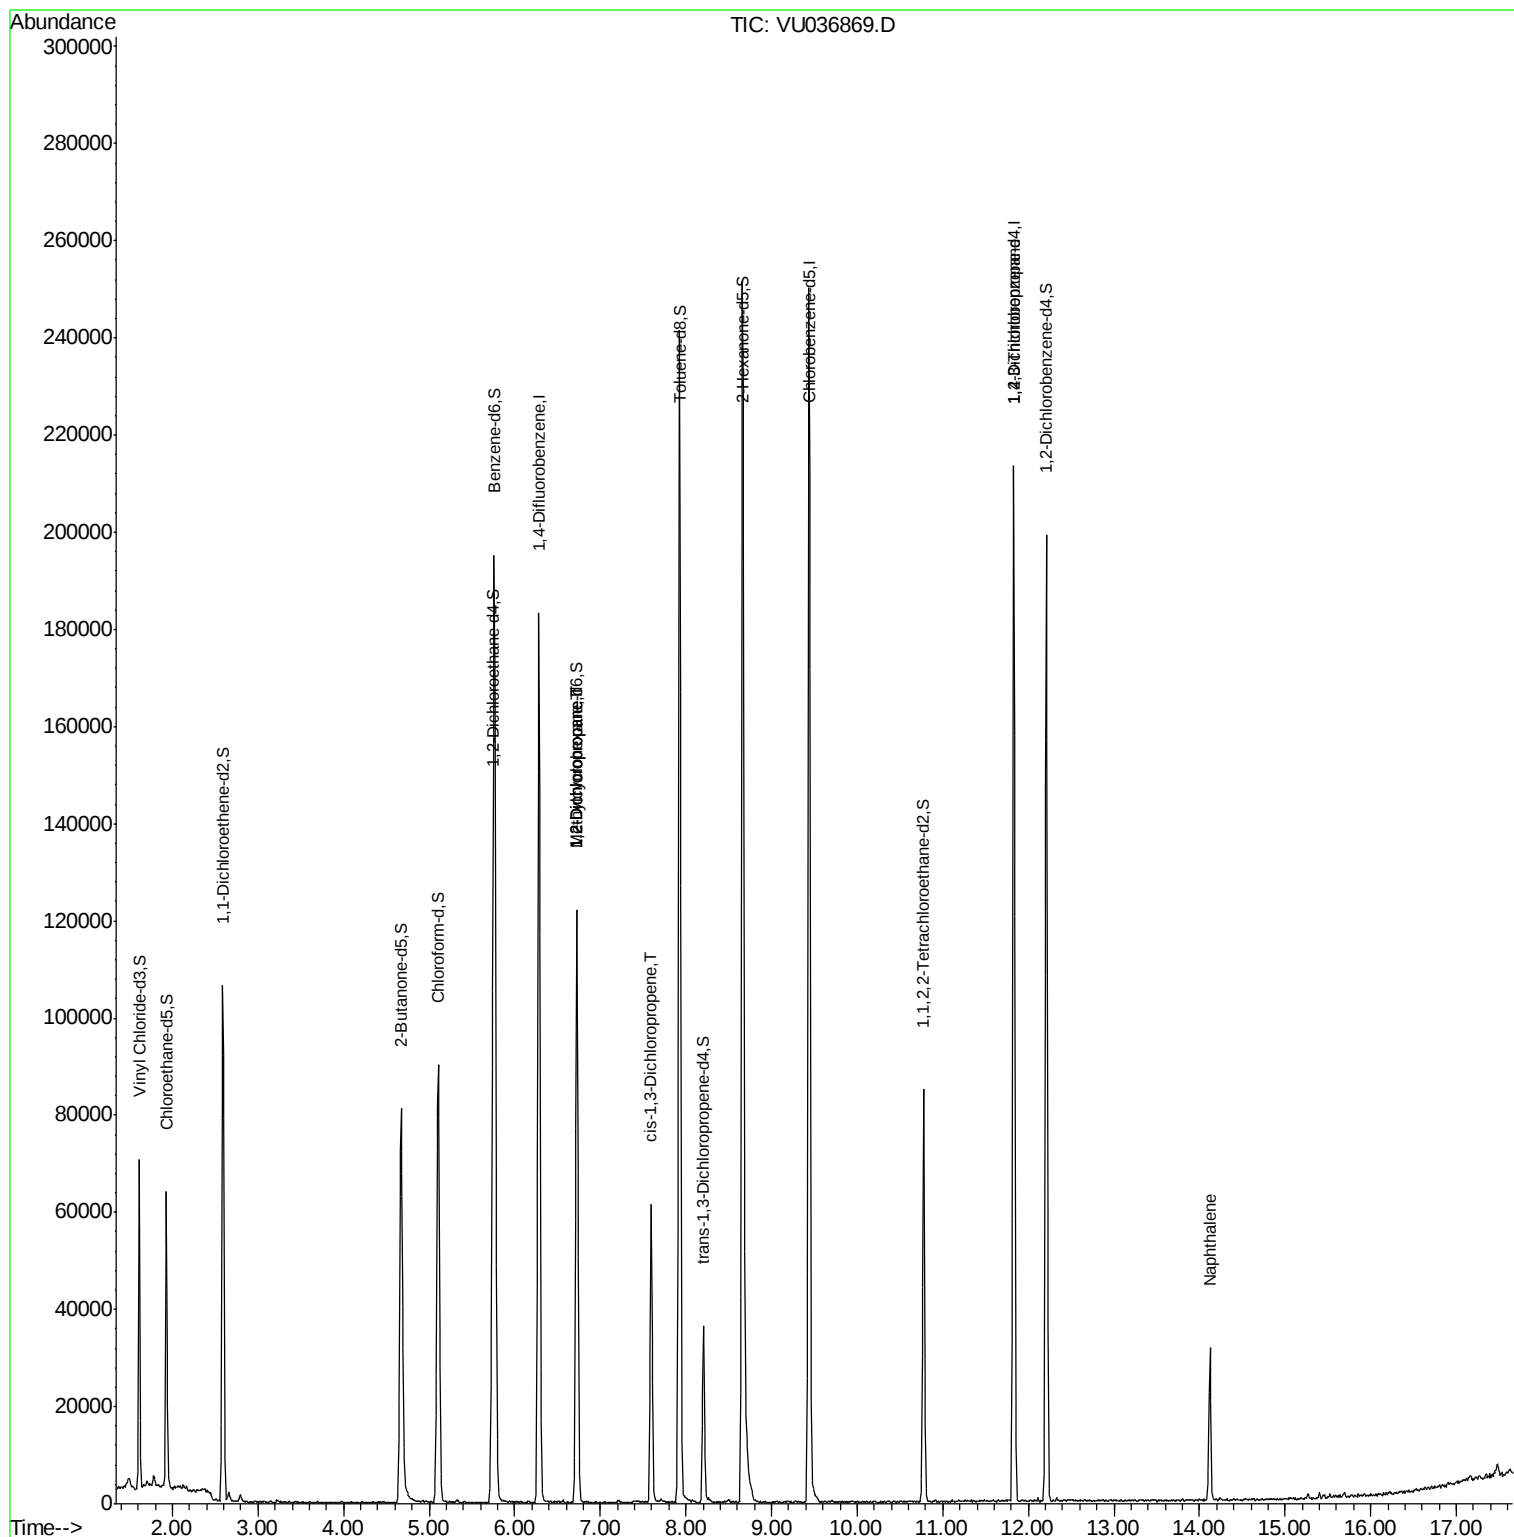


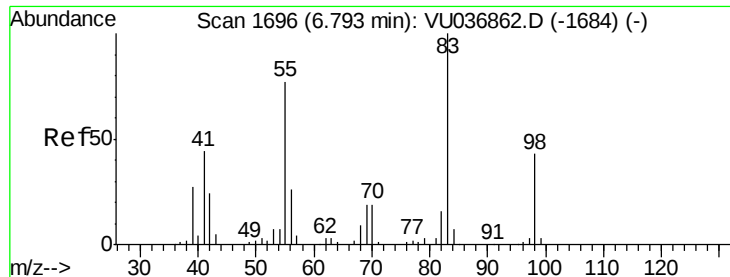




#35
Methylcyclohexane
Concen: 0.751 ug/L
RT: 6.73 min Scan# 1675
Delta R.T. -0.07 min
Lab File: VU036869.D
Acq: 20 Feb 2020 15:27

Instrument :
MSVOA_U
ClientSampleId :
DBDW4

Tgt Ion: 83 Resp: 12517
Ion Ratio Lower Upper
83 100
55 0.0 61.0 91.4#
98 0.4 34.2 51.4#

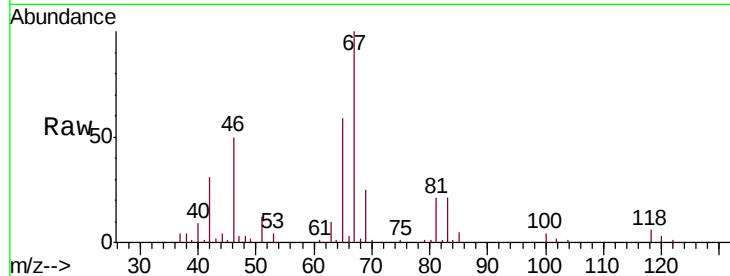


Abundance Ion 83.15 (82.85 to 83.85): VU0
Ion 55.10 (54.80 to 55.80): VU0
Ion 98.15 (97.85 to 98.85): VU0

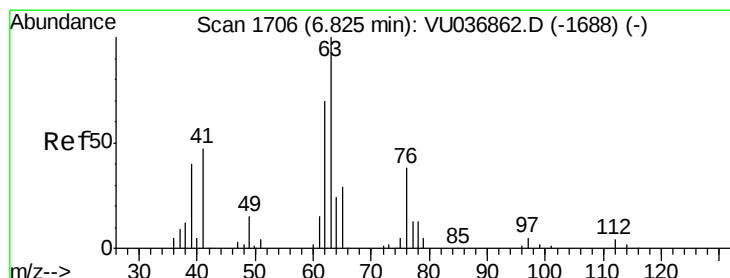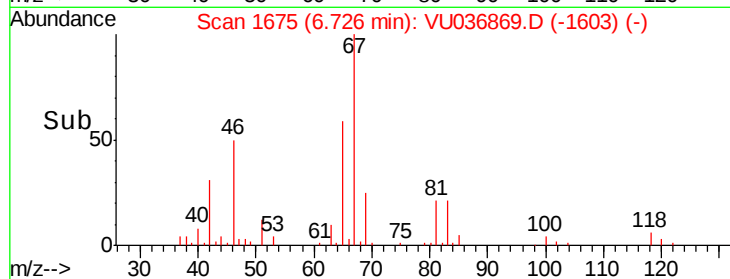
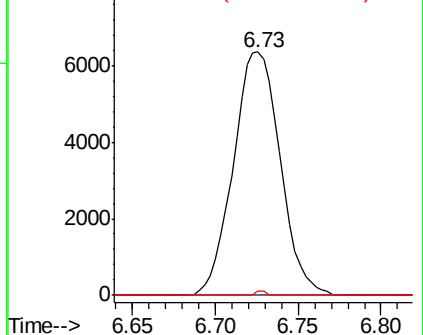



#37
1,2-Dichloropropane
Concen: 0.545 ug/L
RT: 6.73 min Scan# 1675
Delta R.T. -0.10 min
Lab File: VU036869.D
Acq: 20 Feb 2020 15:27

Tgt Ion: 63 Resp: 6137
Ion Ratio Lower Upper
63 100
112 0.0 3.0 4.4#

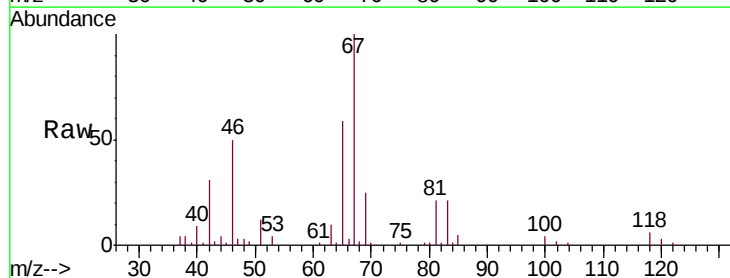

Abundance Ion 63.10 (62.80 to 63.80): VU0
Ion 112.10 (111.80 to 112.80): V



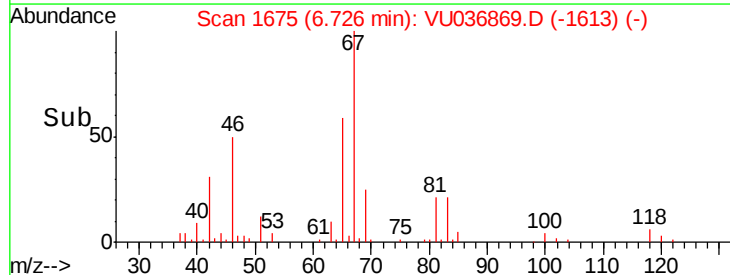
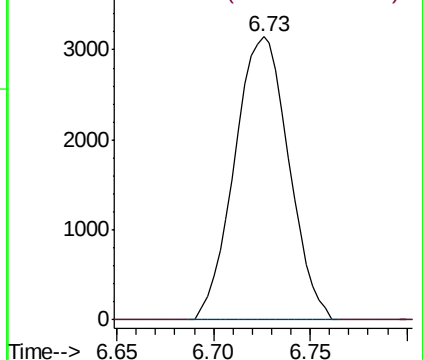


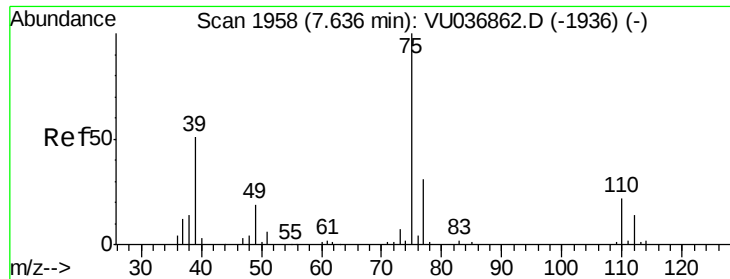

#39
 cis-1,3-Dichloropropene
 Concen: 0.089 ug/L
 RT: 7.60 min Scan# 1946
 Delta R.T. -0.04 min
 Lab File: VU036869.D
 Acq: 20 Feb 2020 15:27




Instrument :
 MSVOA_U
 ClientSampleId :
 DBDW4


Tgt Ion: 75 Resp: 1442
 Ion Ratio Lower Upper
 75 100
 77 58.7 22.5 41.9#

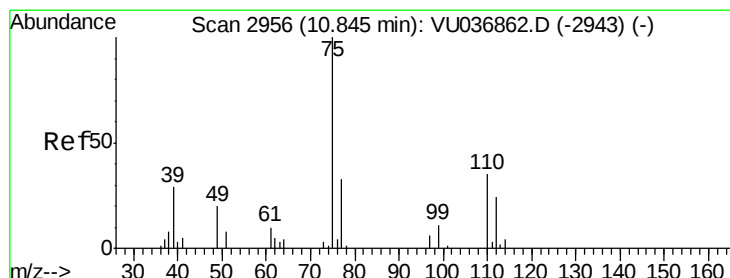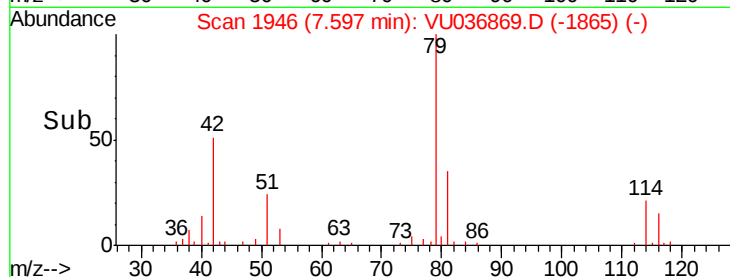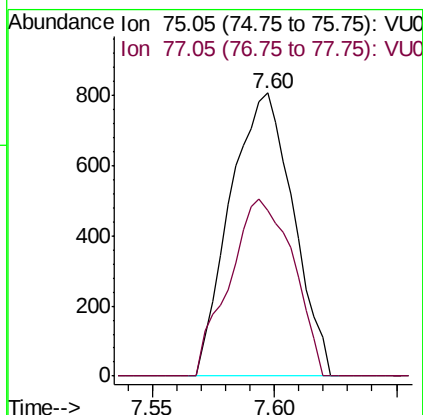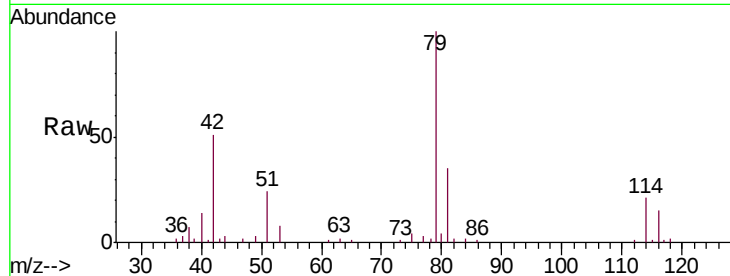

#59
 1,2,3-Trichloropropane
 Concen: 1.068 ug/L
 RT: 11.83 min Scan# 3262
 Delta R.T. 0.98 min
 Lab File: VU036869.D
 Acq: 20 Feb 2020 15:27

Tgt Ion: 75 Resp: 7938
 Ion Ratio Lower Upper
 75 100
 77 36.3 25.6 38.4

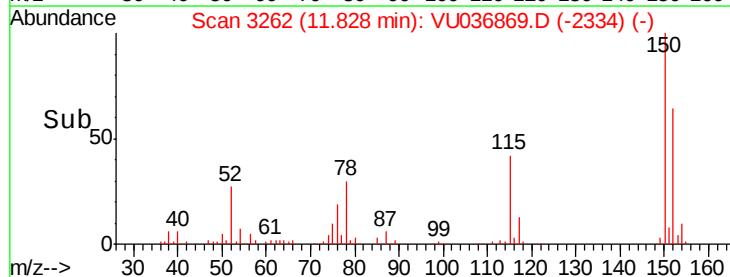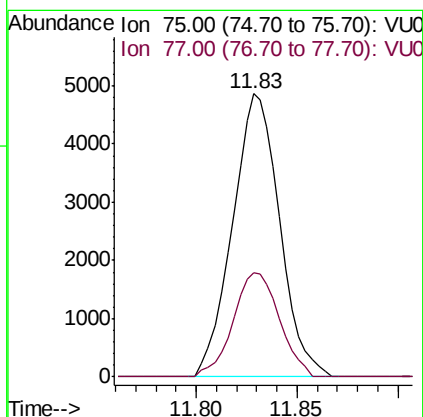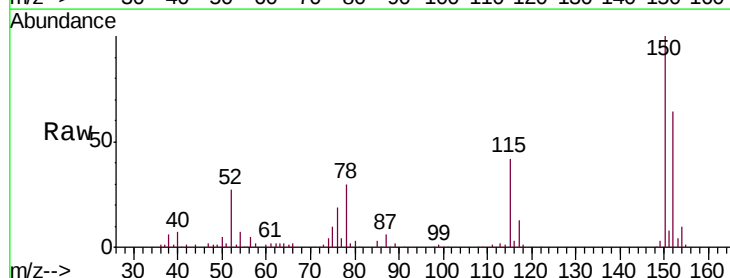

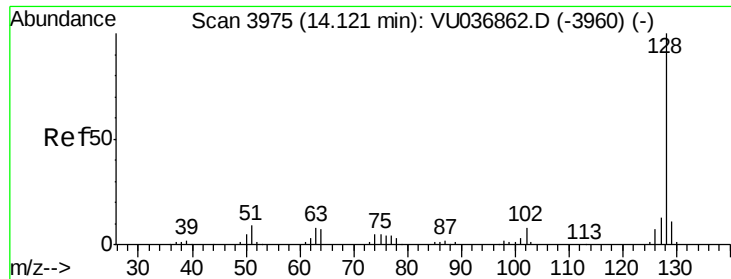

#69

Naphthalene

Concen: 1.435 ug/L

RT: 14.12 min Scan# 3975

Delta R.T. 0.00 min

Lab File: VU036869.D

Acq: 20 Feb 2020 15:27

Instrument :

MSVOA_U

ClientSampleId :

DBDW4


Tgt Ion:128 Resp: 24833

Ion Ratio Lower Upper

128 100

129 10.9 9.0 13.4

127 12.5 10.8 16.2

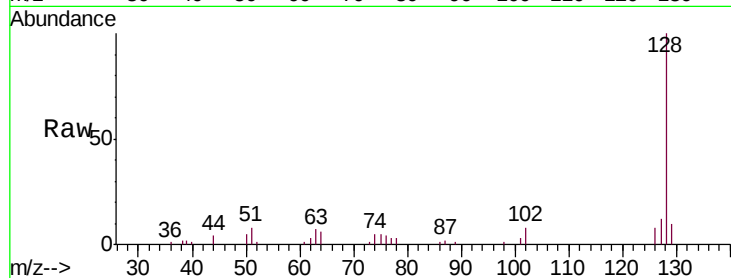

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 127.00 (126.70 to 127.70): V

