

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU022020\
 Data File : VU036868.D
 Acq On : 20 Feb 2020 15:03
 Operator : JC/MD
 Sample : L1580-19
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBDW3

Quant Time: Feb 21 01:15:39 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Feb 21 00:49:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	131301	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	122855	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	50618	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	44319	3.92	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.40%
7) Chloroethane-d5	1.93	69	42806	4.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.40%
11) 1,1-Dichloroethene-d2	2.59	63	64400	3.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.20%
20) 2-Butanone-d5	4.69	46	123468	52.14	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.28%
24) Chloroform-d	5.11	84	81252	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
26) 1,2-Dichloroethane-d4	5.74	65	46156	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%
32) Benzene-d6	5.76	84	174942	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.60%
36) 1,2-Dichloropropane-d6	6.73	67	55319	4.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.40%
41) Toluene-d8	7.92	98	156113	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.80%
43) trans-1,3-Dichloropropene-	8.21	79	19052	4.13	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.60%
46) 2-Hexanone-d5	8.66	63	103654	49.26	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.52%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	41915	4.48	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.60%
64) 1,2-Dichlorobenzene-d4	12.21	152	49366	4.88	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.60%


Target Compounds					Ovalue
13) Acetone	2.68	43	2941	0.971 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU022020\
Data File : VU036868.D
Acq On : 20 Feb 2020 15:03
Operator : JC/MD
Sample : L1580-19
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBDW3

Quant Time: Feb 21 01:15:39 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Feb 21 00:49:14 2020
Response via : Initial Calibration

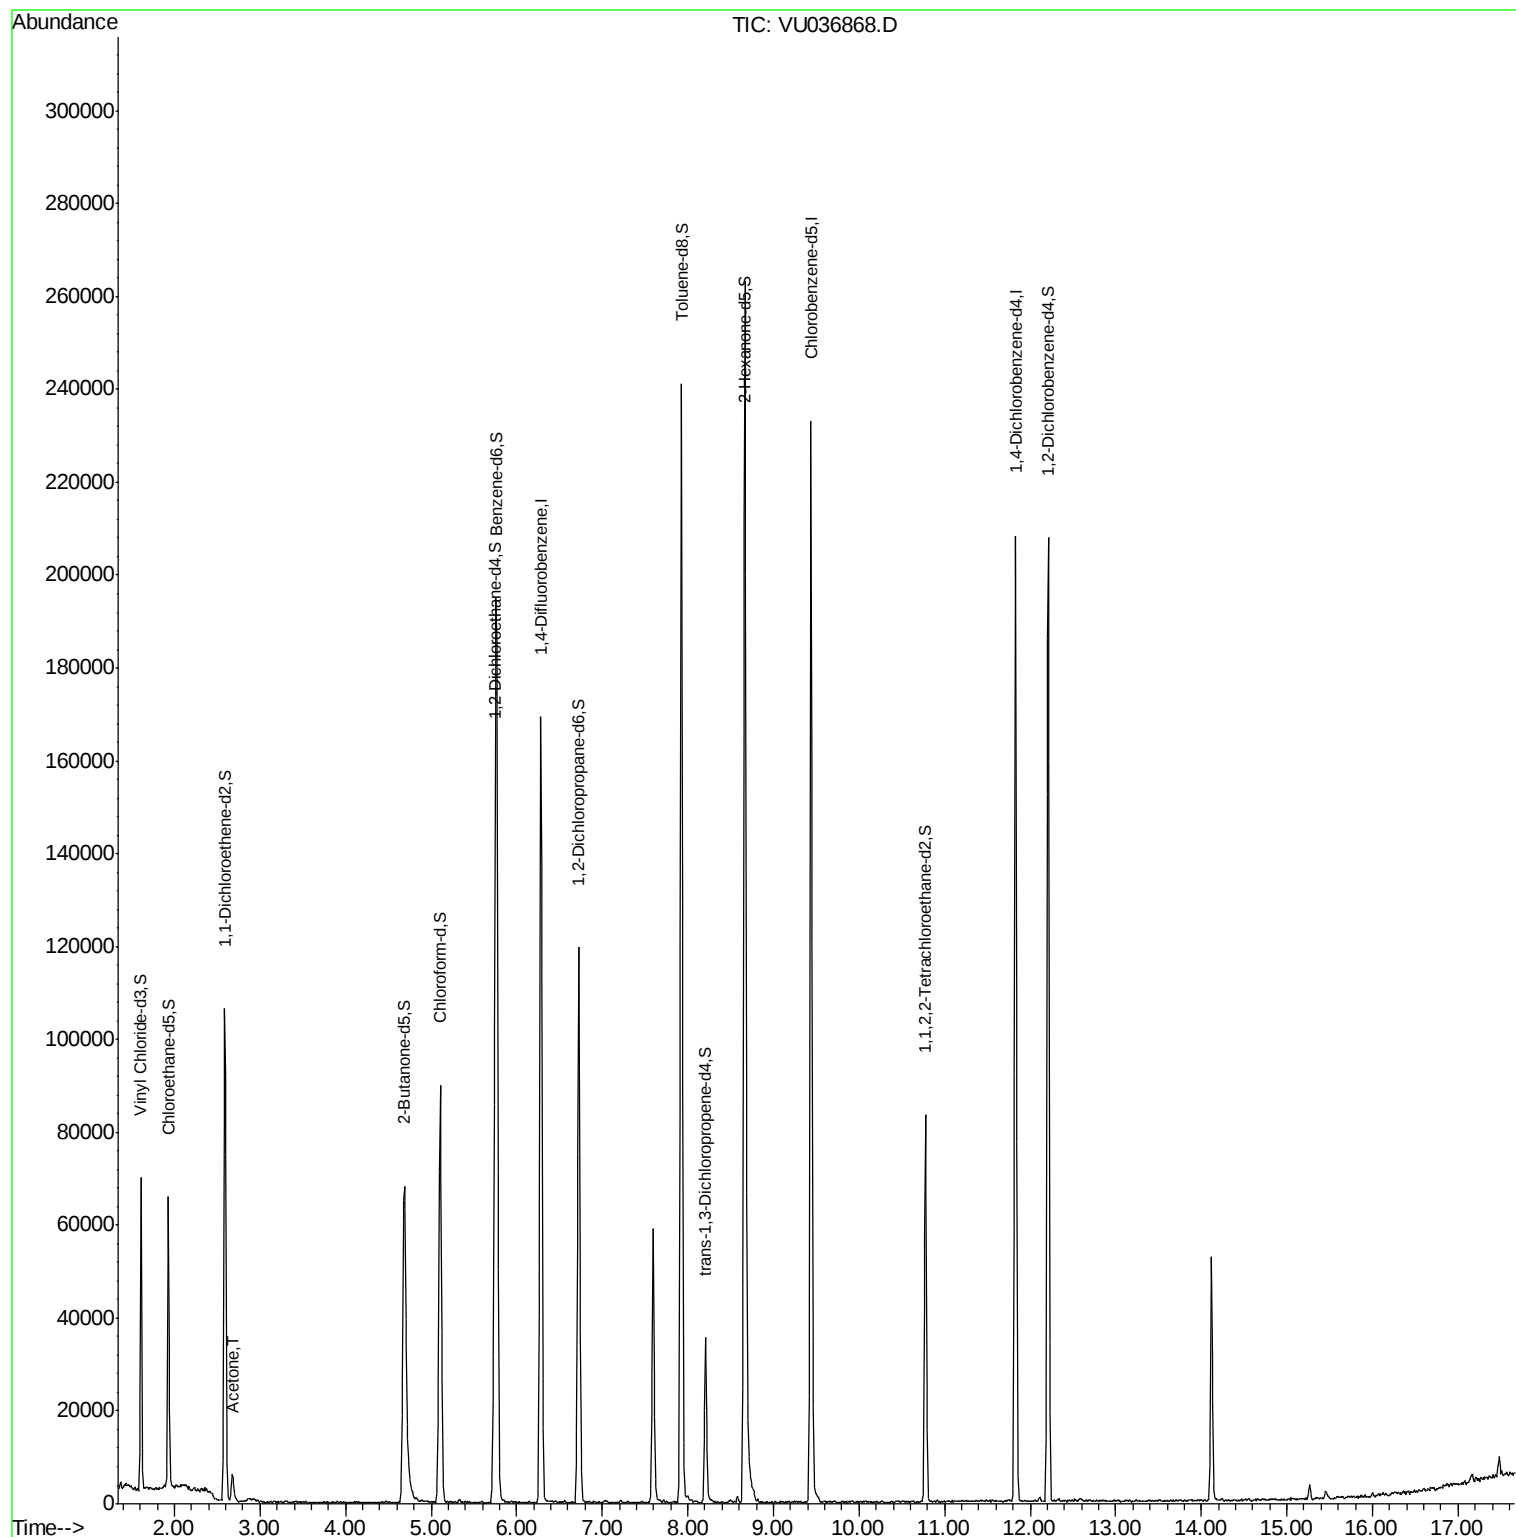

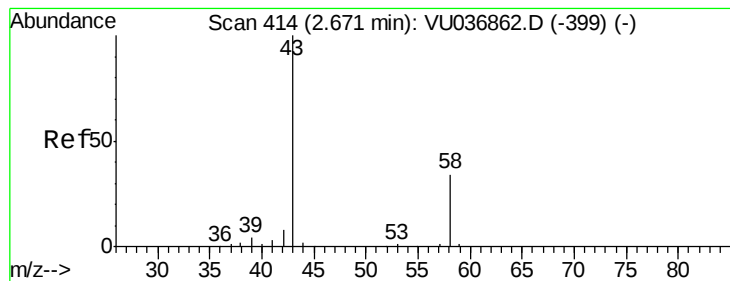

#13
 Acetone
 Concen: 0.971 ug/L
 RT: 2.68 min Scan# 418
 Delta R.T. 0.01 min
 Lab File: VU036868.D
 Acq: 20 Feb 2020 15:03

Instrument :
 MSVOA_U
 ClientSampleId :
 DBDW3

Tot Ion: 43 Resp: 2941
 Ion Ratio Lower Upper
 43 100
 58 31.1 0.0 64.2

