


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU022020\
 Data File : VU036861.D
 Acq On : 20 Feb 2020 09:14
 Operator : JC/MD
 Sample : BFB11
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB11

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Feb 21 00:49:14 2020

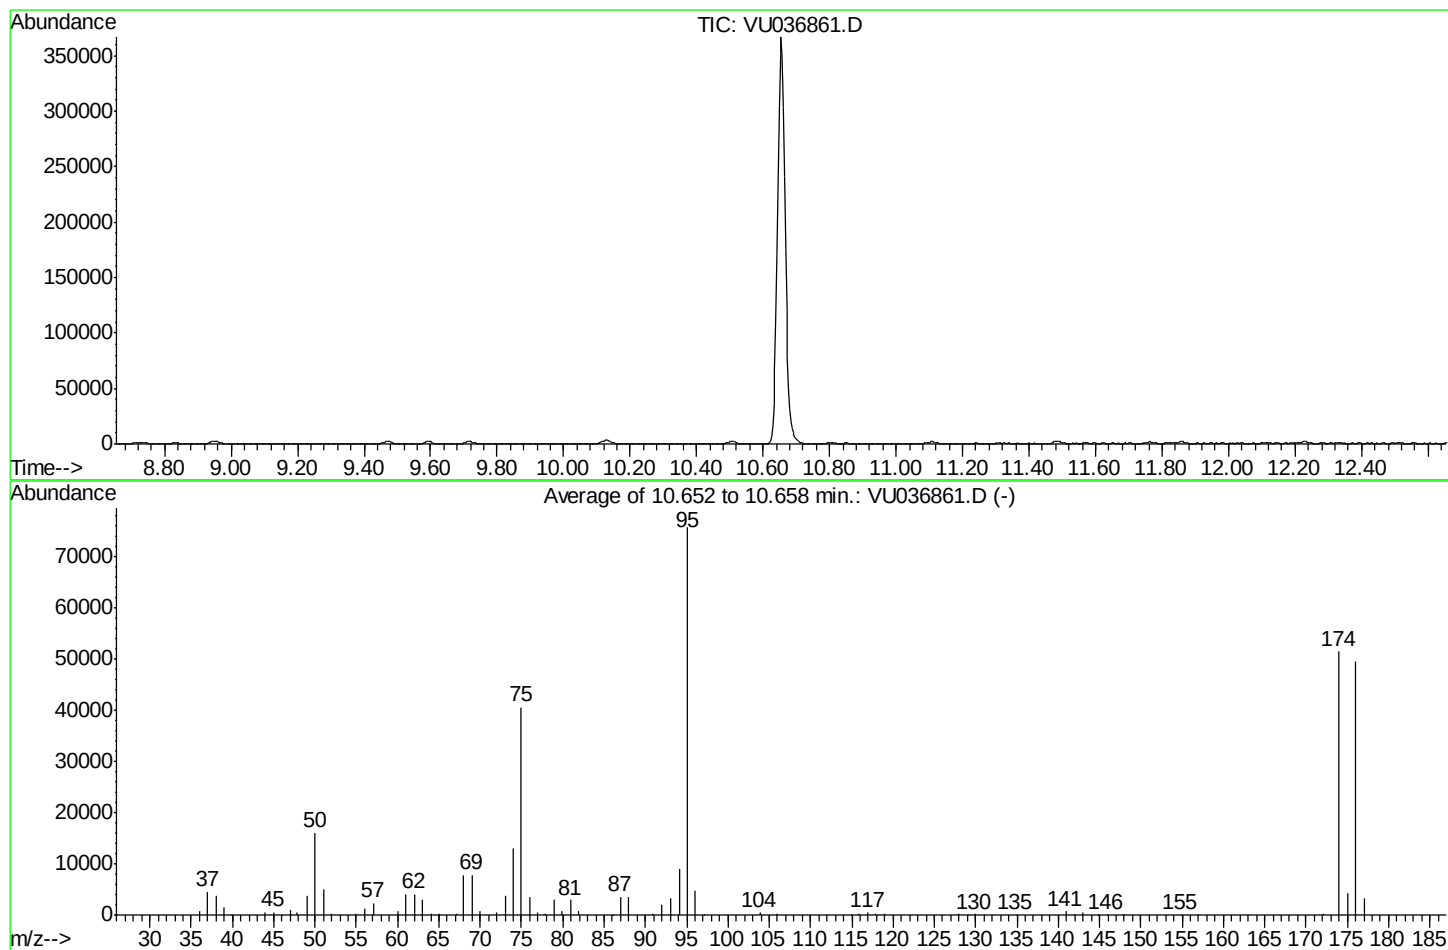

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	16080	PASS
75	95	30	80	53.5	40485	PASS
95	95	100	100	100.0	75658	PASS
96	95	5	9	6.2	4708	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.9	51373	PASS
175	174	5	9	8.1	4180	PASS
176	174	95	101	96.2	49437	PASS
177	176	5	9	6.7	3299	PASS

m/z	Abundance
35.90	788.0
37.00	4588.0
38.00	3764.0
39.00	1558.0
39.90	169.0
44.00	905.0
45.00	610.0
46.00	100.0
46.90	962.0
47.90	612.0
49.00	4023.0
50.00	16030.0
51.00	4993.0
52.00	169.0
55.00	229.0
56.00	1378.0
57.00	2287.0
60.00	908.0
61.00	3992.0
62.00	3958.0
63.00	2951.0
64.00	293.0
65.00	201.0
67.10	331.0
68.00	7888.0
69.00	7823.0
70.00	739.0
72.00	509.0
73.00	3627.0
74.00	13193.0
75.00	40600.0
76.00	3337.0
76.90	381.0
77.90	313.0
78.90	2932.0
79.90	757.0
80.90	2840.0
81.90	594.0
87.00	3606.0
88.00	3461.0
90.90	358.0
92.00	2078.0
93.00	3272.0
94.10	8898.0
95.10	75272.0
96.10	4597.0
97.10	123.0
103.90	341.0
106.00	328.0
115.90	239.0
117.00	462.0
117.90	228.0
119.00	392.0
127.90	189.0
128.90	104.0
130.00	227.0
131.00	108.0
134.90	105.0
140.90	607.0
141.90	112.0
143.00	583.0
145.90	100.0
147.80	122.0
154.90	128.0
172.10	303.0
174.00	49360.0
175.10	4146.0
176.00	46968.0
177.00	3315.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

m/z	Abundance
35.00	905.0
37.00	4667.0
38.00	3851.0
39.00	1545.0
39.00	142.0
44.00	876.0
45.00	583.0
45.00	115.0
46.00	1019.0
47.00	615.0
49.00	3876.0
50.00	16632.0
51.00	4986.0
52.00	193.0
55.00	237.0
56.00	1371.0
57.00	2282.0
60.00	860.0
61.00	4017.0
62.00	4197.0
63.00	3149.0
64.00	390.0
65.00	168.0
68.00	7953.0
69.00	7962.0
70.00	720.0
72.00	532.0
73.00	3827.0
74.10	13383.0
75.00	41832.0
76.00	3628.0
77.00	449.0
77.00	380.0
78.00	2962.0
80.00	709.0
80.00	2999.0
82.00	673.0
87.00	3695.0
88.00	3557.0
90.00	356.0
92.00	2127.0
93.00	3284.0
94.10	9258.0
95.10	78256.0
96.00	4865.0
97.10	135.0
103.00	408.0
106.00	367.0
115.80	221.0
117.00	425.0
117.00	258.0
119.00	377.0
127.00	217.0
129.00	105.0
130.00	220.0
131.00	117.0
134.00	116.0
140.00	691.0
143.00	610.0
144.00	101.0
145.00	119.0
148.00	138.0
154.00	131.0
156.00	119.0
172.10	351.0
174.00	52864.0
175.00	4297.0
176.00	51024.0
177.00	3422.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

m/z	Abundance
36.00	909.0
37.00	4251.0
38.00	3601.0
39.00	1446.0
39.80	126.0
44.00	825.0
45.00	595.0
45.90	131.0
47.00	1004.0
47.80	554.0
49.00	3471.0
50.00	15578.0
51.00	4664.0
52.00	209.0
55.00	230.0
56.00	1256.0
57.10	2206.0
60.00	789.0
61.00	3678.0
62.00	4044.0
63.00	3110.0
64.00	411.0
65.00	131.0
67.10	198.0
68.00	7252.0
69.00	7691.0
70.00	658.0
72.00	479.0
73.00	3588.0
74.00	12649.0
75.00	39024.0
76.00	3541.0
76.90	464.0
77.90	410.0
78.90	2759.0
80.00	653.0
80.90	2828.0
82.00	678.0
86.10	134.0
87.00	3451.0
88.00	3374.0
90.90	309.0
92.00	1917.0
93.00	3118.0
94.10	8821.0
95.10	73448.0
96.00	4662.0
97.10	136.0
103.90	414.0
106.00	311.0
114.90	101.0
115.80	204.0
117.00	369.0
117.90	253.0
119.00	311.0
127.90	234.0
129.00	104.0
129.90	222.0
134.90	113.0
140.90	720.0
143.00	591.0
145.90	119.0
148.00	136.0
154.90	106.0
157.00	123.0
172.00	341.0
174.00	51896.0
175.00	4097.0
176.00	50320.0
177.00	3162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

Scan 2883 (10.610 min): VU036861.D
BFB11

m/z	Abundance
40.00	124.0
43.90	303.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11