

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022021\
 Data File : VU042364.D
 Acq On : 19 Feb 2021 16:12
 Operator : SY/MD
 Sample : M1404-01 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 NWB-1579-1582

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U021721W.M

Title : SW846 8260

Signal : TIC: VU042364.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.694	100	110	150	rBV	559975	828462	100.00%	16.089%
2	2.366	301	319	321	rBV2	8730	19632	2.37%	0.381%
3	2.649	393	407	422	rBV	7249	15963	1.93%	0.310%
4	4.655	1017	1031	1048	rBV3	4699	15118	1.82%	0.294%
5	5.298	1215	1231	1245	rBV	126652	272684	32.91%	5.295%
6	5.382	1245	1257	1277	rVB	222901	457989	55.28%	8.894%
7	5.713	1344	1360	1383	rBV	140639	296285	35.76%	5.754%
8	6.259	1515	1530	1549	rBV	294610	570367	68.85%	11.076%
9	7.906	2028	2042	2071	rBV	451326	798986	96.44%	15.516%
10	9.426	2502	2515	2536	rBV	402338	675098	81.49%	13.110%
11	10.642	2880	2893	2916	rVB	333004	548943	66.26%	10.660%
12	11.819	3247	3259	3276	rBV	404381	649837	78.44%	12.620%




Sum of corrected areas: 5149364

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022021\
Data File : VU042364.D
Acq On : 19 Feb 2021 16:12
Operator : SY/MD
Sample : M1404-01 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
NWB-1579-1582

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U021721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

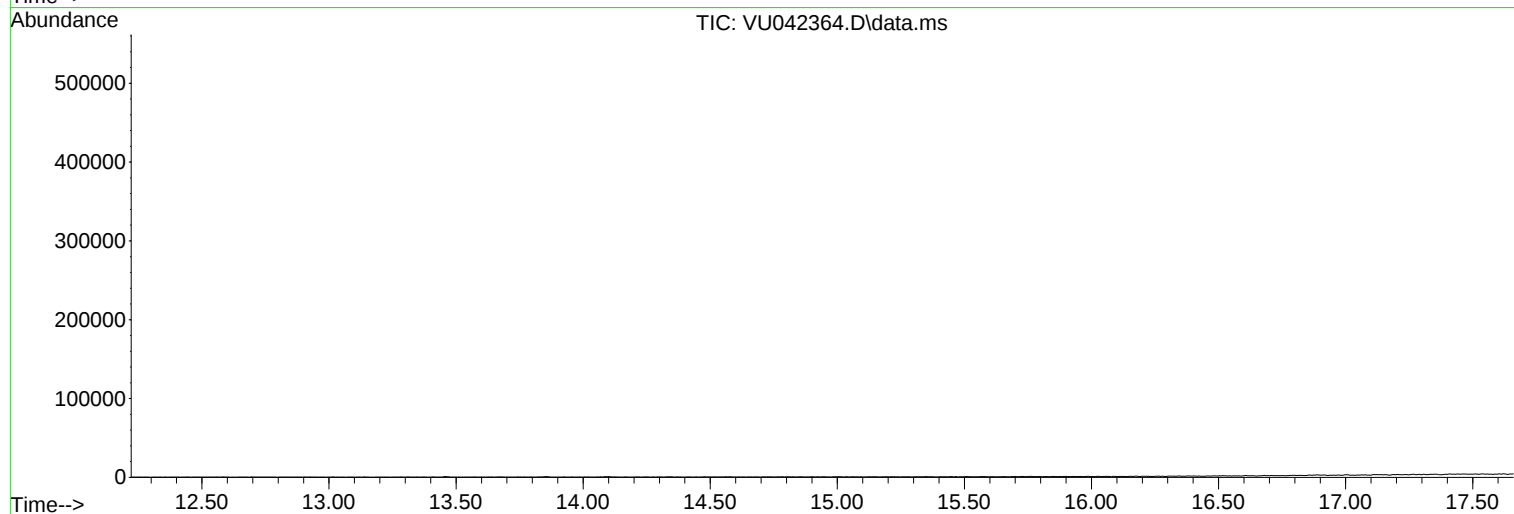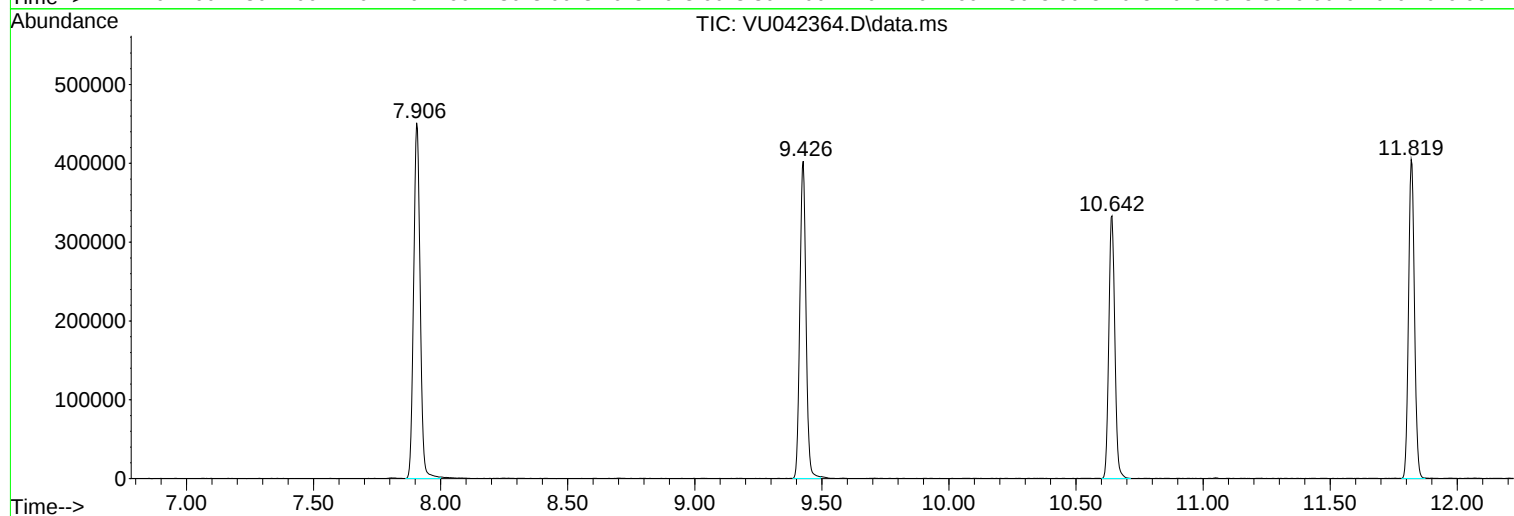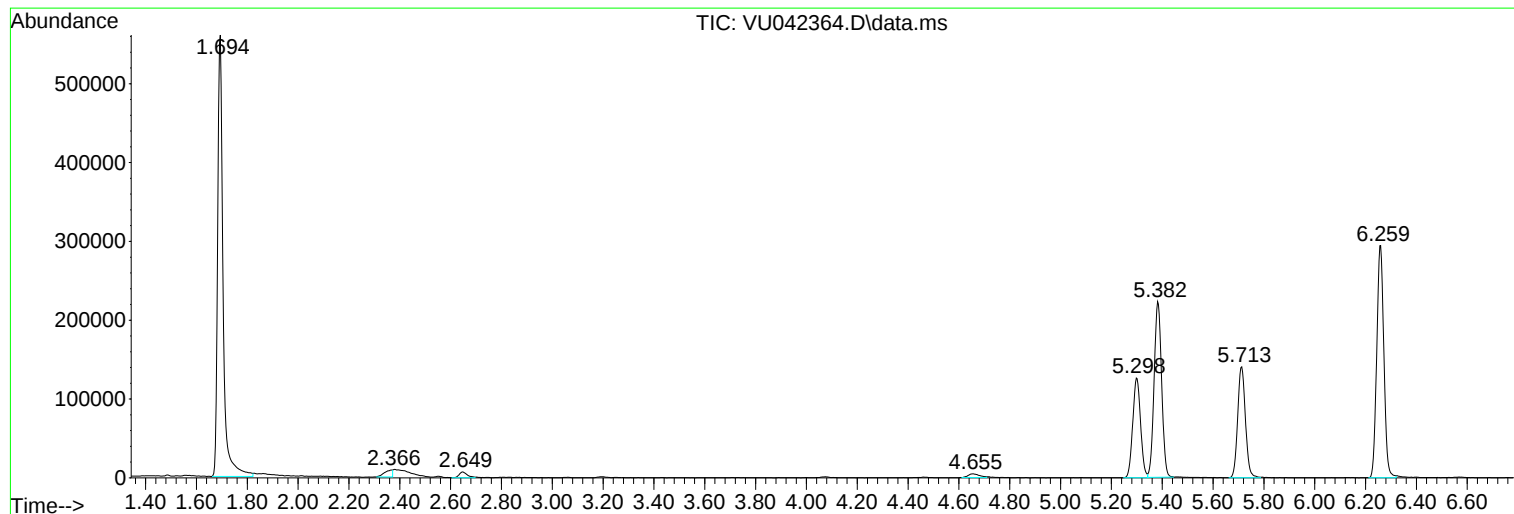

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022021\
Data File : VU042364.D
Acq On : 19 Feb 2021 16:12
Operator : SY/MD
Sample : M1404-01 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
NWB-1579-1582










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U021721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.694 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.694	90.45 ug/l	828462	Pentafluorobenzene	5.385

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Acetaldehyde	44	C2H4O	000075-07-0	9
2			Propane	44	C3H8	000074-98-6	5
3			Ethylene oxide	44	C2H4O	000075-21-8	5
4			Carbon dioxide	44	CO2	000124-38-9	3
5			Ethyne, fluoro-	44	C2HF	002713-09-9	3

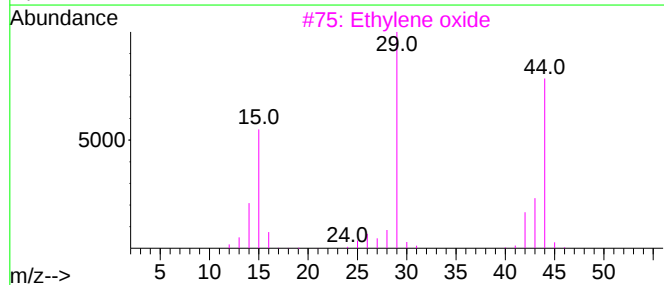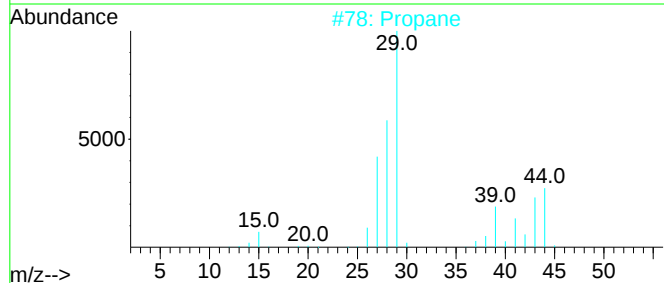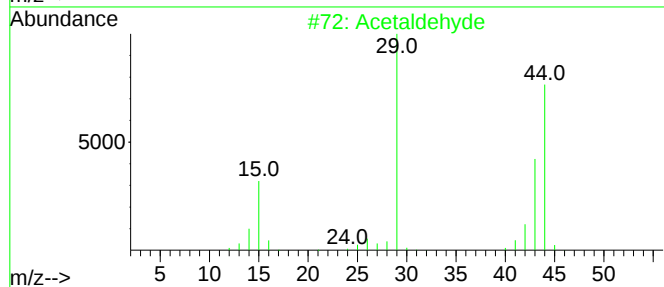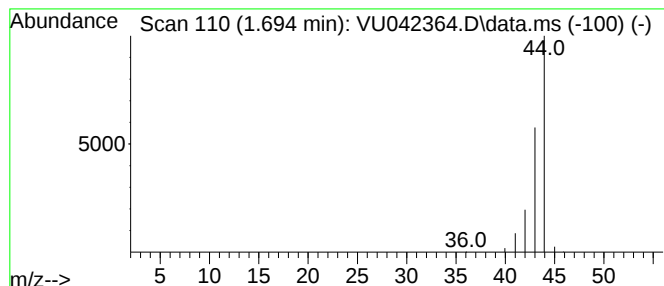

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022021\
Data File : VU042364.D
Acq On : 19 Feb 2021 16:12
Operator : SY/MD
Sample : M1404-01 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
NWB-1579-1582

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U021721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.694	1.694	90.5	ug/l	828462	1	5.385	457989	50.0