
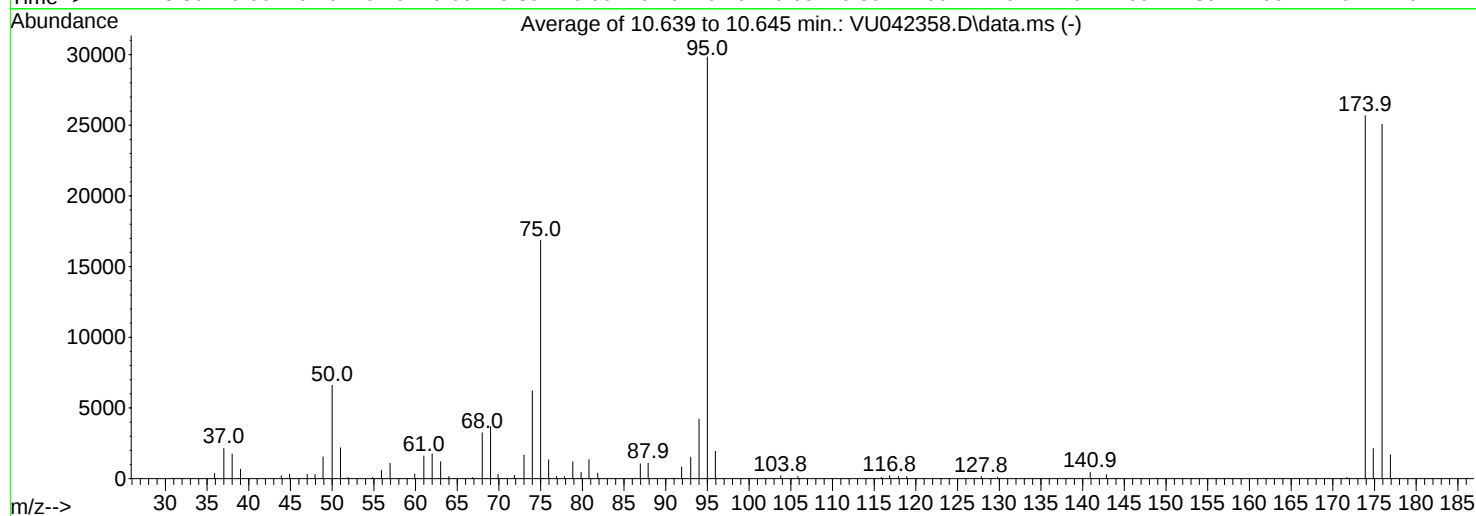


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022021\
Data File : VU042358.D
Acq On : 19 Feb 2021 13:09
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U021721W.M
Title : SW846 8260
Last Update : Fri Feb 19 02:55:52 2021

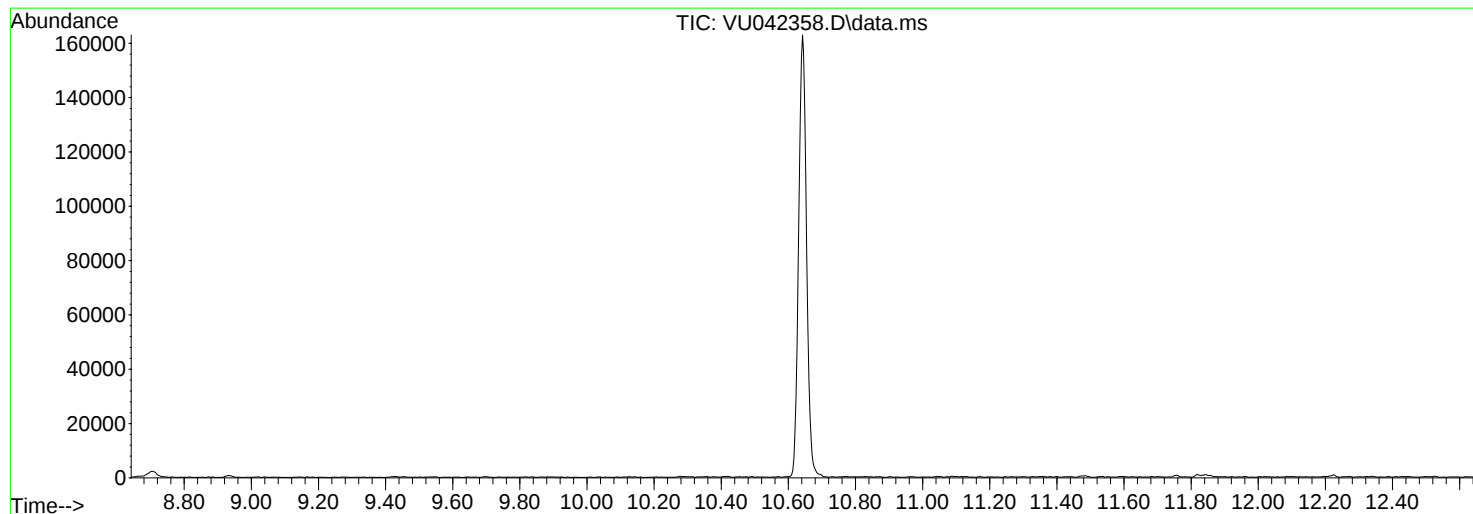

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	6594	PASS
75	95	30	60	56.5	16850	PASS
95	95	100	100	100.0	29840	PASS
96	95	5	9	6.5	1938	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.1	25688	PASS
175	174	5	9	8.3	2123	PASS
176	174	95	101	97.5	25056	PASS
177	176	5	9	6.7	1685	PASS