


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022023\
Data File : VU053139.D
Acq On : 20 Feb 2023 08:50
Operator : JC/MD
Sample : BFB199
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB199

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sun Feb 19 23:26:18 2023

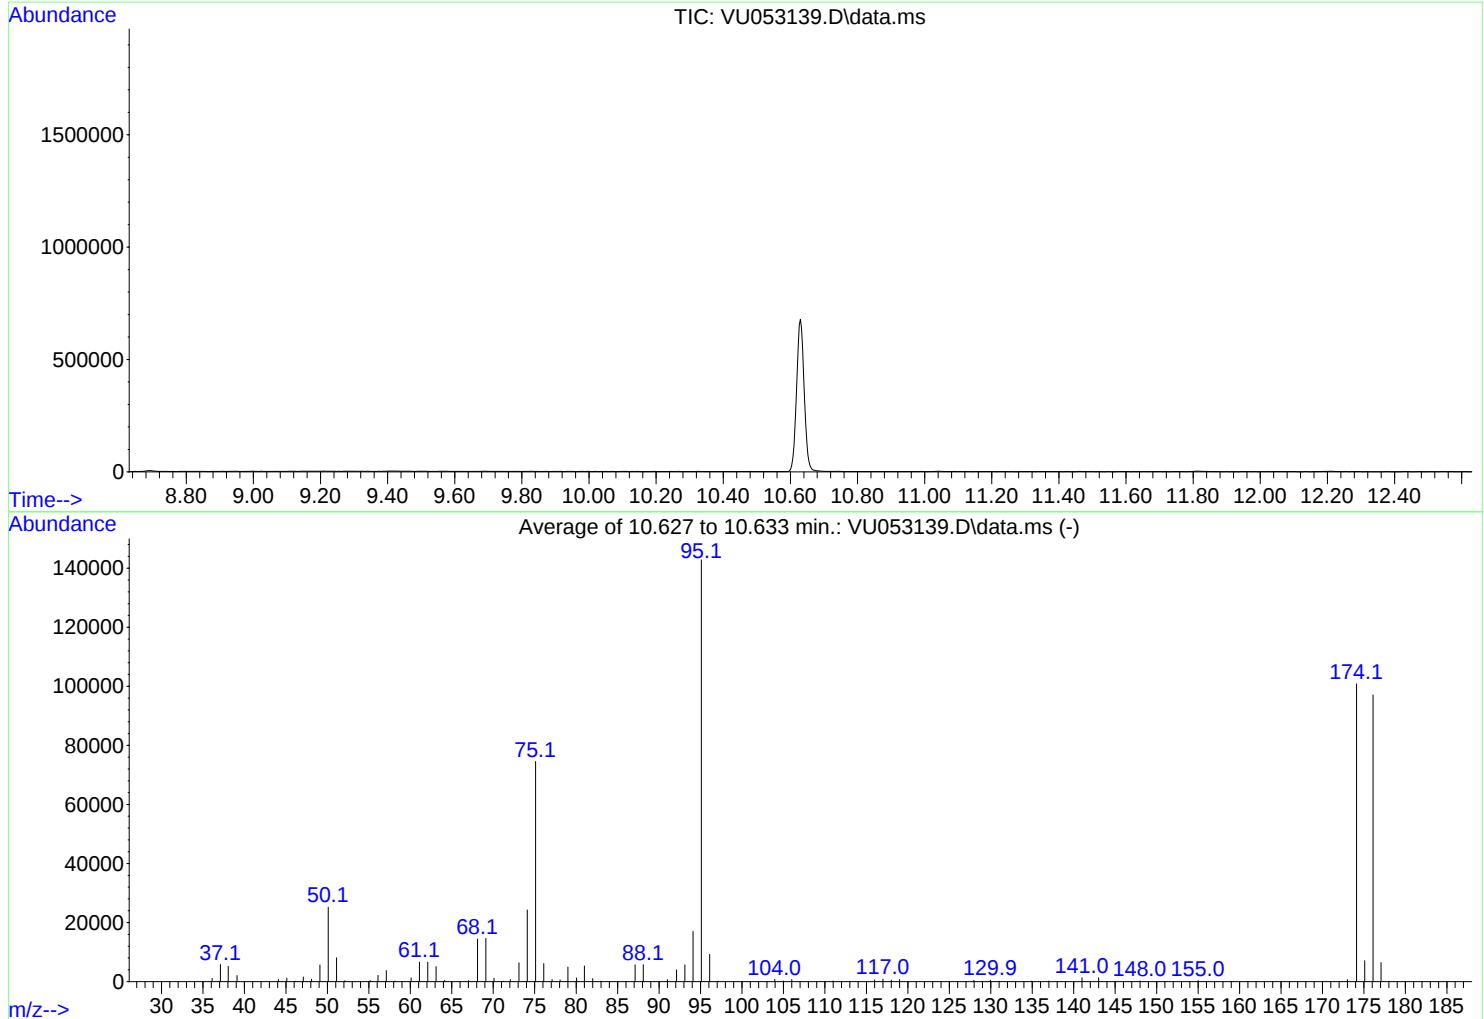

AutoFind: Scans 2966, 2967, 2968; Background Corrected with Scan 2951

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.6	25205	PASS
75	95	30	80	52.2	74563	PASS
95	95	100	100	100.0	142827	PASS
96	95	5	9	6.5	9219	PASS
173	174	0.00	2	0.7	673	PASS
174	95	50	120	70.6	100840	PASS
175	174	5	9	7.0	7102	PASS
176	174	95	101	96.3	97099	PASS
177	176	5	9	6.7	6478	PASS