


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022023\
 Data File : VU053139.D
 Acq On : 20 Feb 2023 08:50
 Operator : JC/MD
 Sample : BFB199
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB199

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sun Feb 19 23:26:18 2023

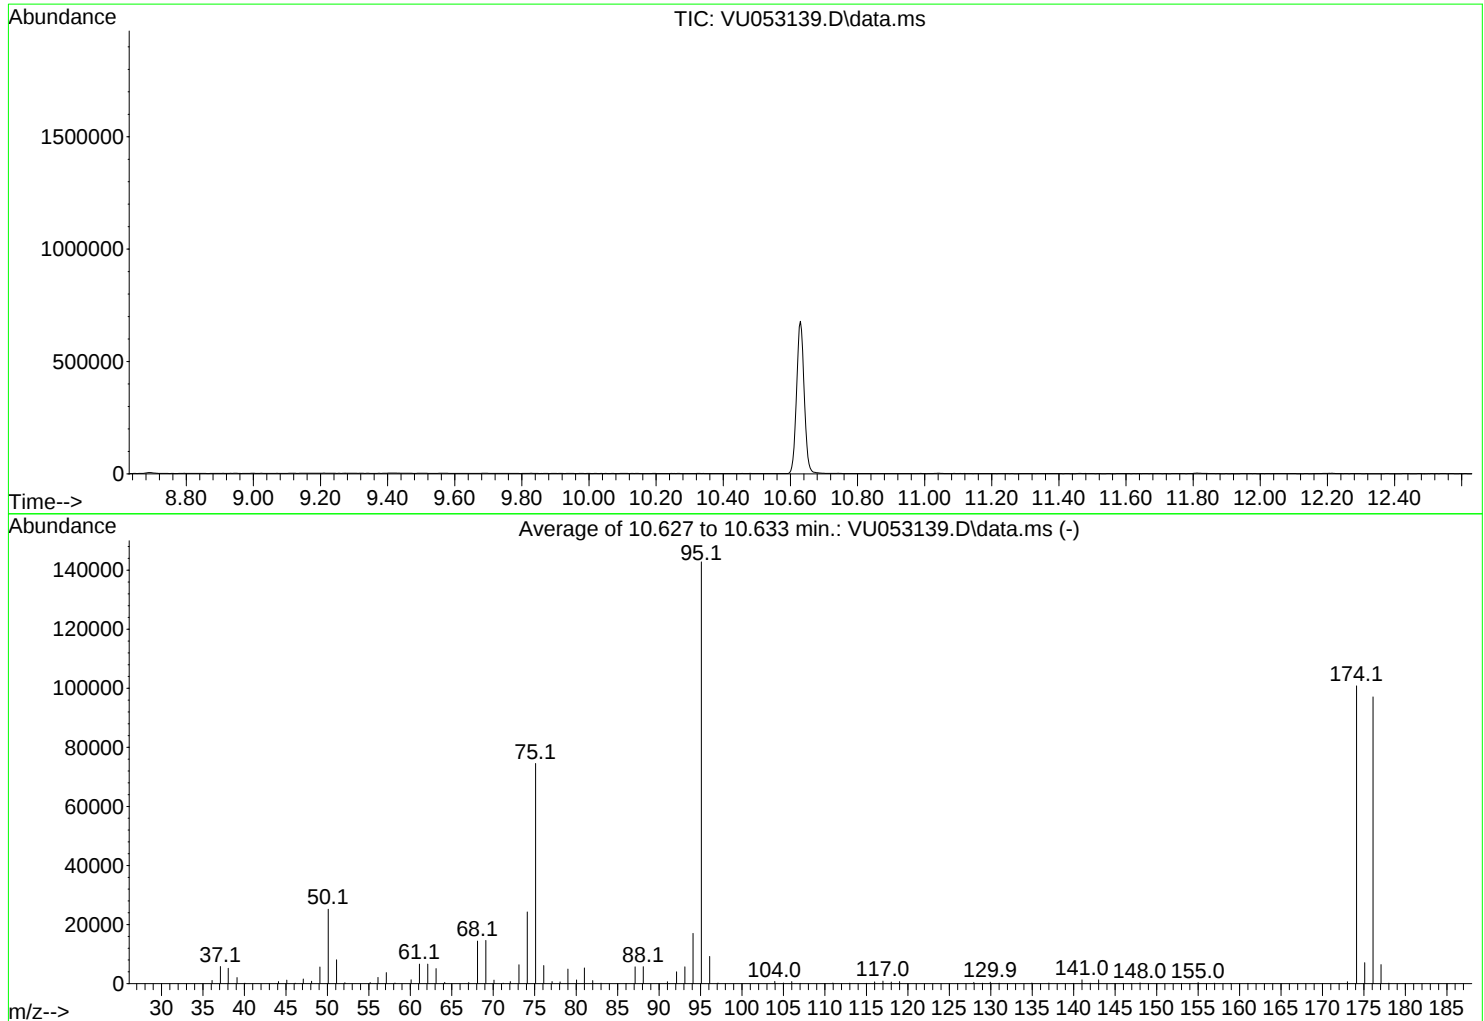

AutoFind: Scans 2966, 2967, 2968; Background Corrected with Scan 2951

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	25205	PASS
75	95	30	80	52.2	74563	PASS
95	95	100	100	100.0	142827	PASS
96	95	5	9	6.5	9219	PASS
173	174	0.00	2	0.7	673	PASS
174	95	50	120	70.6	100840	PASS
175	174	5	9	7.0	7102	PASS
176	174	95	101	96.3	97099	PASS
177	176	5	9	6.7	6478	PASS

m/z	Abundance
35.10	156.0
36.10	769.0
38.00	318.0
41.00	101.0
44.10	195.0

Instrument :
MSVOA_U
ClientSampleId :
BFB199

m/z	Abundance
35.10	233.0
36.10	1938.0
37.10	5985.0
38.10	5700.0
39.10	2072.0
40.00	133.0
44.10	937.0
45.10	1200.0
46.10	147.0
47.10	1631.0
48.10	914.0
49.10	5914.0
50.10	25632.0
51.10	8095.0
52.10	317.0
55.10	387.0
56.10	2165.0
57.10	3876.0
58.20	254.0
60.10	1257.0
61.10	6586.0
62.10	6524.0
63.10	5198.0
64.10	434.0
67.10	378.0
68.10	14425.0
69.10	14943.0
70.10	1267.0
71.20	167.0
72.00	705.0
73.10	6496.0
74.10	24240.0
75.10	74656.0
76.10	6308.0
77.10	752.0
78.10	558.0
79.00	5131.0
80.10	1249.0
81.00	5246.0
82.00	1066.0
83.00	141.0
87.10	5821.0
88.10	5709.0
91.00	679.0
92.10	4052.0
93.10	5586.0
94.10	17424.0
95.10	142336.0
96.10	9329.0
97.10	221.0
104.00	731.0
105.00	193.0
106.00	732.0
107.00	140.0
110.00	104.0
111.00	191.0
113.00	162.0
115.00	146.0
116.00	581.0
117.00	879.0
118.00	537.0
119.00	666.0
126.00	106.0
128.00	432.0
129.00	169.0
129.90	457.0
131.00	191.0
135.00	208.0
137.00	236.0
140.00	118.0
141.00	1342.0
142.00	156.0
143.00	1269.0
145.00	131.0
145.90	158.0
146.90	103.0
148.00	235.0
153.00	154.0
155.00	347.0
157.00	191.0
158.90	113.0
173.00	604.0
174.10	97320.0
175.10	7183.0
176.10	94848.0
177.00	6385.0
178.00	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB199

m/z	Abundance
36.10	1870.0
37.10	5905.0
38.10	5770.0
39.10	2090.0
40.00	153.0
43.00	107.0
44.10	913.0
45.10	1249.0
46.10	156.0
47.10	1622.0
48.10	839.0
49.10	5851.0
50.10	26128.0
51.10	8245.0
52.10	372.0
55.10	379.0
56.10	2148.0
57.10	3829.0
58.20	236.0
60.10	1368.0
61.10	6825.0
62.10	6762.0
63.10	5247.0
64.10	453.0
67.10	398.0
68.10	14918.0
69.10	15140.0
70.10	1247.0
71.20	154.0
72.10	694.0
73.10	6587.0
74.10	25096.0
75.10	77088.0
76.10	6339.0
77.10	684.0
78.00	631.0
79.00	5037.0
80.00	1240.0
81.00	5525.0
82.00	1043.0
83.00	174.0
86.10	104.0
87.10	5888.0
88.10	5961.0
91.00	668.0
92.10	4130.0
93.10	5903.0
94.10	17608.0
95.10	147712.0
96.10	9520.0
97.10	238.0
103.90	790.0
105.00	232.0
106.00	710.0
107.00	133.0
110.00	110.0
111.00	214.0
113.00	167.0
115.00	128.0
116.00	649.0
117.00	867.0
118.00	546.0
119.00	710.0
126.00	100.0
128.00	448.0
129.00	185.0
130.00	482.0
131.00	151.0
135.00	217.0
137.00	239.0
140.00	130.0
141.00	1369.0
142.00	163.0
143.00	1328.0
145.00	125.0
145.90	134.0
146.90	121.0
148.00	279.0
153.00	156.0
155.00	382.0
157.00	179.0
158.90	129.0
161.00	124.0
172.10	108.0
173.00	681.0
174.10	104256.0
175.10	7243.0
176.10	100256.0
177.10	6661.0
178.00	158.0

Instrument :
MSVOA_U
ClientSampleId :
BFB199

m/z	Abundance
36.10	1719.0
37.10	5459.0
38.10	5144.0
39.10	2005.0
40.10	172.0
41.10	116.0
43.00	142.0
44.10	838.0
45.10	1107.0
46.10	134.0
47.10	1454.0
48.10	665.0
49.10	5215.0
50.10	23856.0
51.10	7833.0
52.10	355.0
55.20	347.0
56.10	2018.0
57.10	3468.0
58.10	175.0
60.10	1349.0
61.10	6424.0
62.10	6543.0
63.10	4785.0
64.20	466.0
67.00	383.0
68.10	13877.0
69.10	13834.0
70.10	1093.0
71.20	113.0
72.10	677.0
73.10	6145.0
74.10	23448.0
75.10	71944.0
76.10	5784.0
77.10	665.0
78.00	586.0
79.00	4689.0
80.00	1231.0
81.00	5157.0
82.00	987.0
83.00	175.0
86.00	121.0
87.10	5402.0
88.10	5590.0
91.00	603.0
92.10	3888.0
93.10	5596.0
94.10	15956.0
95.10	138432.0
96.10	8808.0
97.10	228.0
103.90	749.0
105.00	214.0
106.00	597.0
107.10	112.0
110.90	196.0
113.00	171.0
116.00	647.0
117.00	835.0
118.00	536.0
119.00	697.0
127.90	470.0
129.00	198.0
130.00	456.0
131.00	151.0
134.90	237.0
137.00	220.0
139.90	108.0
141.00	1278.0
142.00	130.0
143.00	1334.0
146.00	112.0
146.90	110.0
148.00	293.0
150.00	105.0
153.00	113.0
155.00	353.0
156.90	164.0
158.90	132.0
161.00	163.0
171.90	140.0
173.00	735.0
174.10	100944.0
175.10	6879.0
176.10	96192.0
177.10	6389.0
178.00	141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB199