

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057905.D
 Acq On : 20 Feb 2024 16:18
 Operator : MD/SY
 Sample : P1513-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Feb 21 00:15:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 21 00:11:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	299951	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	280050	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	130022	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	94466	43.501	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	87.000%		
7) Chloroethane-d5	1.907	69	74932	46.685	ug/L	0.02
Spiked Amount 50.000	Range 70 - 130		Recovery =	93.360%		
11) 1,1-Dichloroethene-d2	2.560	63	131636	32.527	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.060%		
21) 2-Butanone-d5	4.608	46	94038	113.973	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	113.970%		
24) Chloroform-d	5.052	84	169559	46.047	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.100%		
26) 1,2-Dichloroethane-d4	5.692	65	112763	48.851	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.700%		
32) Benzene-d6	5.717	84	351566	50.093	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.180%		
36) 1,2-Dichloropropane-d6	6.682	67	112790	49.771	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	99.540%		
41) Toluene-d8	7.891	98	314024	49.429	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.860%		
43) trans-1,3-Dichloroprop...	8.174	79	51129	47.378	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.760%		
47) 2-Hexanone-d5	8.624	63	73948	84.880	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	84.880%		
56) 1,1,2,2-Tetrachloroeth...	10.749	84	136999	43.810	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.620%		
66) 1,2-Dichlorobenzene-d4	12.187	152	103400	49.113	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.220%		
Target Compounds						Qvalue
60) 1,2,3-Trichloropropane	11.804	75	17458	5.795	ug/L	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057905.D
Acq On : 20 Feb 2024 16:18
Operator : MD/SY
Sample : P1513-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Feb 21 00:15:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 21 00:11:26 2024
Response via : Initial Calibration

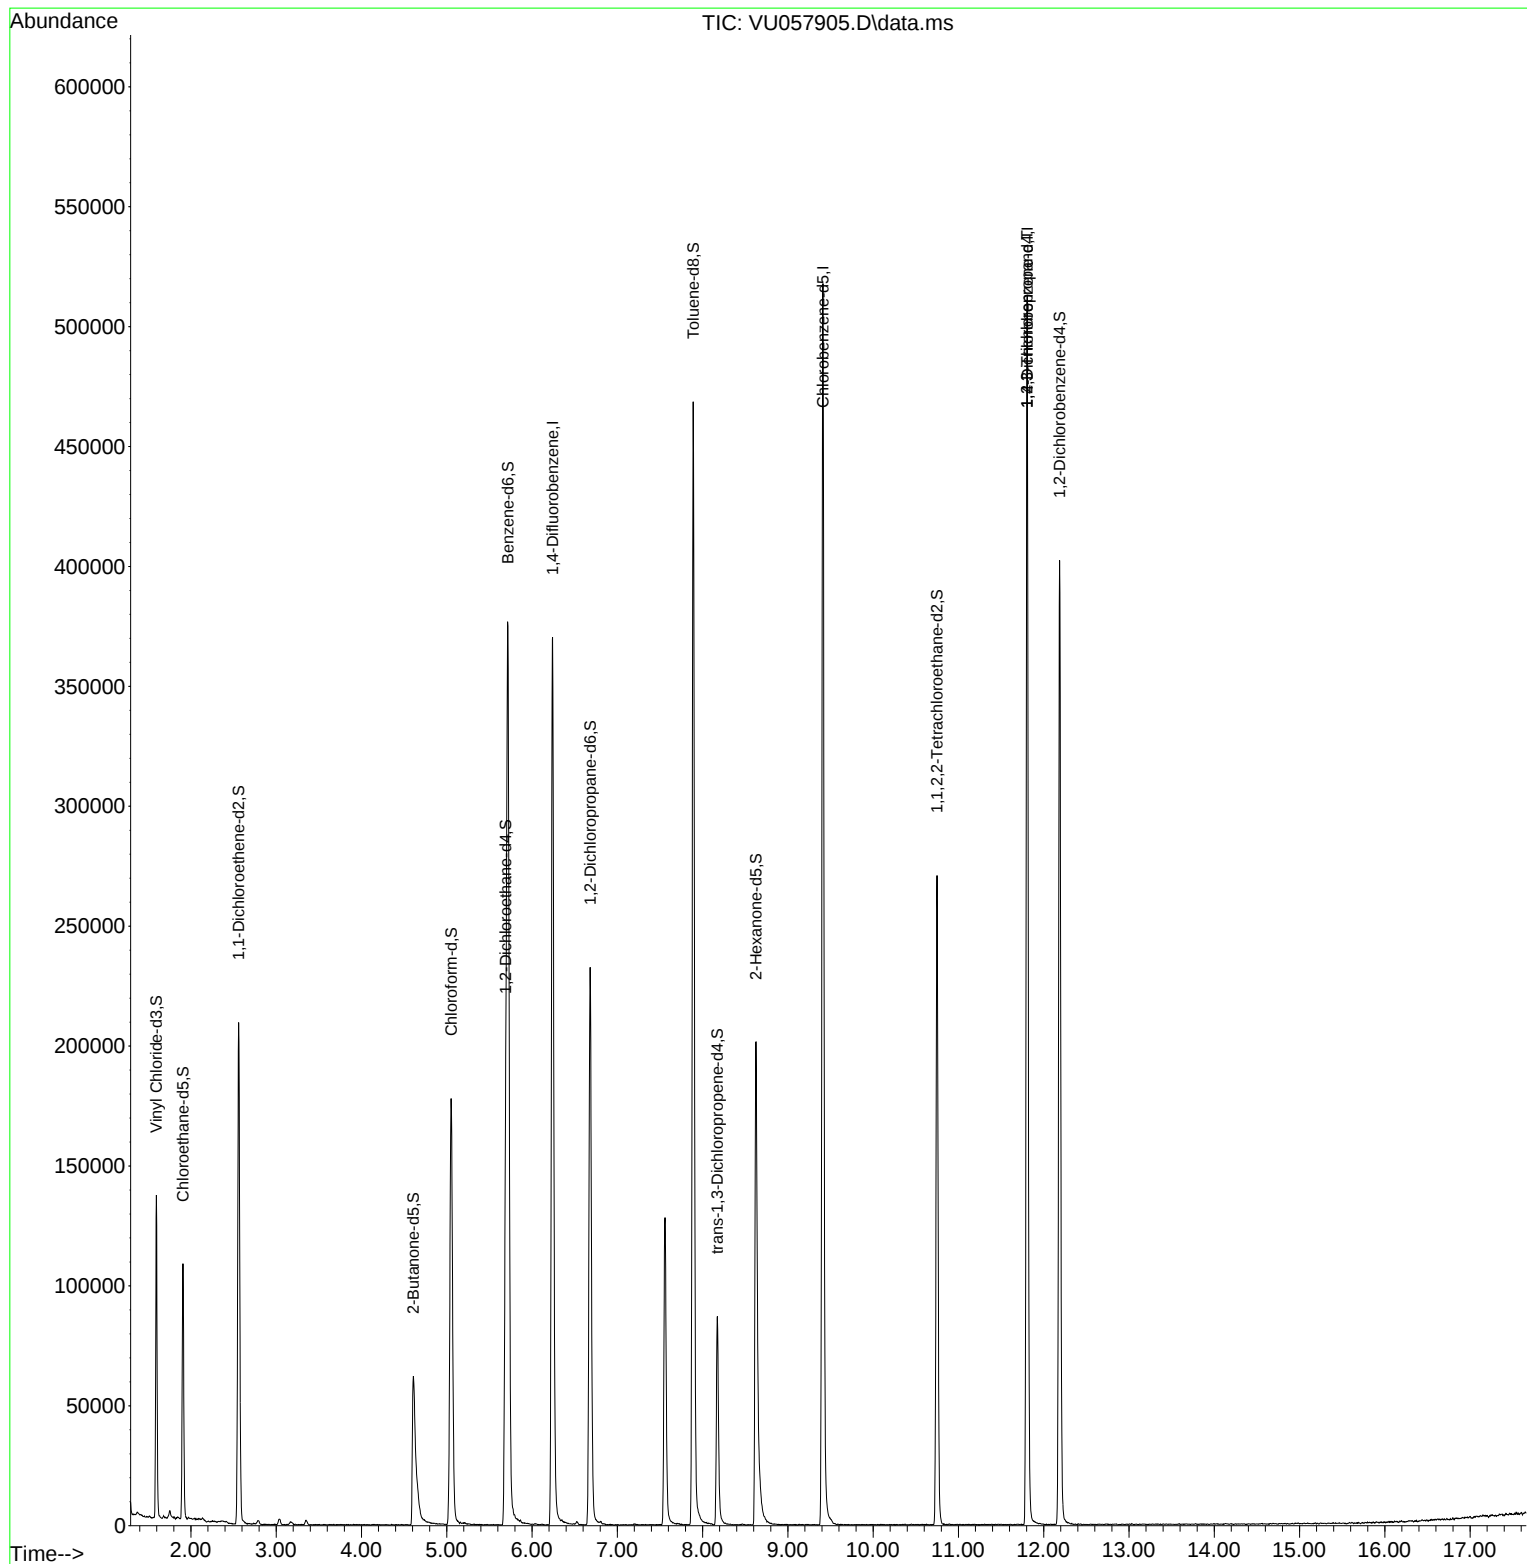

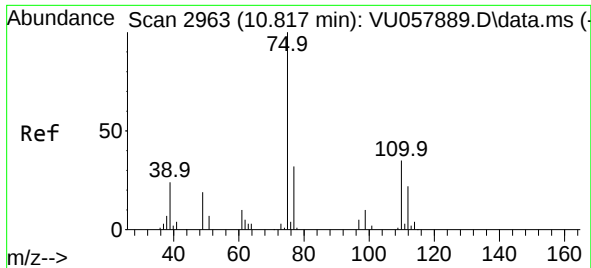

#60
 1,2,3-Trichloropropane
 Concen: 5.795 ug/L
 RT: 11.804 min Scan# 31
 Delta R.T. 0.987 min
 Lab File: VU057905.D
 Acq: 20 Feb 2024 16:18

Instrument :
 MSVOA_U
 ClientSampleId :

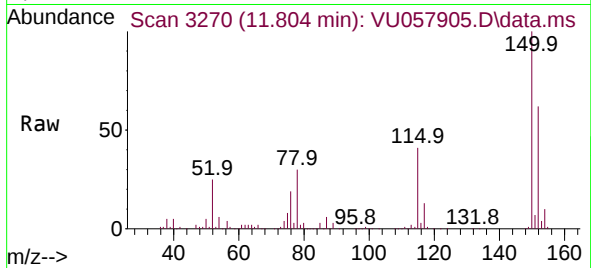

Tgt Ion: 75 Resp: 17458
 Ion Ratio Lower Upper
 75 100
 77 29.8 25.9 38.9
 110 2.4 28.3 42.5#

