

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057890.D
 Acq On : 20 Feb 2024 10:03
 Operator : MD/SY
 Sample : VU0220WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK041

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M

Title : VOC Analysis

Signal : TIC: VU057890.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	113	rBV	124927	148142	15.30%	2.006%
2	1.888	178	186	204	rVB	96410	134737	13.92%	1.824%
3	2.554	381	393	415	rBV	203996	332943	34.39%	4.507%
4	2.705	437	440	442	rBV	255	182	0.02%	0.002%
5	2.782	456	464	471	rBV	988	1519	0.16%	0.021%
6	2.837	478	481	485	rVB2	256	237	0.02%	0.003%
7	2.862	485	489	492	rBV2	247	226	0.02%	0.003%
8	2.933	508	511	513	rBV	321	184	0.02%	0.002%
9	3.033	532	542	552	rBV2	3295	5388	0.56%	0.073%
10	3.129	565	572	575	rBV2	202	312	0.03%	0.004%
11	3.171	575	585	598	rVB4	1466	3258	0.34%	0.044%
12	3.222	598	601	603	rBV2	256	187	0.02%	0.003%
13	3.316	625	630	634	rBV2	226	263	0.03%	0.004%
14	3.341	634	638	639	rBV	354	209	0.02%	0.003%
15	3.502	683	688	691	rBV2	290	329	0.03%	0.004%
16	3.647	729	733	736	rBV2	329	297	0.03%	0.004%
17	3.763	765	769	775	rVV2	162	220	0.02%	0.003%
18	3.981	831	837	840	rBV	400	398	0.04%	0.005%
19	4.010	840	846	850	rVV	283	390	0.04%	0.005%
20	4.036	851	854	866	rVB2	290	567	0.06%	0.008%
21	4.113	874	878	883	rVB2	279	292	0.03%	0.004%
22	4.145	883	888	891	rBV	391	287	0.03%	0.004%
23	4.210	904	908	911	rBV	296	275	0.03%	0.004%
24	4.386	955	963	966	rBV2	178	241	0.02%	0.003%
25	4.608	1022	1032	1059	rBV	57460	149390	15.43%	2.022%
26	4.791	1086	1089	1093	rBV3	335	290	0.03%	0.004%
27	5.049	1153	1169	1197	rBV	166573	367978	38.00%	4.982%
28	5.261	1232	1235	1239	rVB2	307	251	0.03%	0.003%
29	5.322	1242	1254	1266	rBV3	1580	3768	0.39%	0.051%
30	5.550	1321	1325	1329	rVB2	250	204	0.02%	0.003%
31	5.714	1355	1376	1402	rBV2	353294	968238	100.00%	13.108%
32	6.078	1485	1489	1491	rVB3	245	186	0.02%	0.003%
33	6.110	1497	1499	1501	rBV	379	205	0.02%	0.003%
34	6.238	1526	1539	1566	rBV	352570	674942	69.71%	9.137%
35	6.486	1613	1616	1621	rVB2	378	239	0.02%	0.003%
36	6.528	1621	1629	1637	rVB5	1596	2625	0.27%	0.036%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057890.D
 Acq On : 20 Feb 2024 10:03
 Operator : MD/SY
 Sample : VU0220WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK041

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

37	6.586	1642	1647	1648	rBV3	543	412	0.04%	0.006%
38	6.679	1662	1676	1708	rBV	221911	434106	44.83%	5.877%
39	6.994	1766	1774	1777	rBV2	278	332	0.03%	0.004%
40	7.033	1782	1786	1790	rBV2	215	237	0.02%	0.003%
41	7.171	1822	1829	1831	rBV3	339	352	0.04%	0.005%
42	7.193	1831	1836	1839	rVV3	628	720	0.07%	0.010%
43	7.245	1847	1852	1857	rBV2	149	199	0.02%	0.003%
44	7.335	1874	1880	1884	rVB2	208	256	0.03%	0.003%
45	7.383	1884	1895	1900	rBV2	279	636	0.07%	0.009%
46	7.557	1938	1949	1976	rBV	121763	218623	22.58%	2.960%
47	7.660	1977	1981	1982	rBV2	503	382	0.04%	0.005%
48	7.888	2040	2052	2072	rBV	433409	759054	78.40%	10.276%
49	8.171	2125	2140	2168	rBV	80071	142778	14.75%	1.933%
50	8.409	2211	2214	2221	rVB	312	314	0.03%	0.004%
51	8.463	2225	2231	2235	rBV2	423	608	0.06%	0.008%
52	8.553	2254	2259	2260	rBV	241	181	0.02%	0.002%
53	8.627	2267	2282	2321	rBV2	187961	389540	40.23%	5.274%
54	8.830	2342	2345	2350	rVB2	312	242	0.02%	0.003%
55	9.081	2419	2423	2425	rBV2	213	183	0.02%	0.002%
56	9.110	2429	2432	2435	rVB	259	189	0.02%	0.003%
57	9.409	2513	2525	2555	rBV	481733	809203	83.57%	10.955%
58	9.569	2571	2575	2582	rVB3	1031	1214	0.13%	0.016%
59	9.598	2582	2584	2587	rVB	375	207	0.02%	0.003%
60	9.692	2607	2613	2623	rVB5	1133	1859	0.19%	0.025%
61	9.772	2634	2638	2640	rBV2	213	201	0.02%	0.003%
62	9.913	2677	2682	2686	rBV2	202	204	0.02%	0.003%
63	10.103	2736	2741	2742	rBV2	652	542	0.06%	0.007%
64	10.479	2853	2858	2859	rBV2	410	259	0.03%	0.004%
65	10.550	2877	2880	2882	rVB2	263	171	0.02%	0.002%
66	10.602	2891	2896	2900	rVB2	180	171	0.02%	0.002%
67	10.653	2910	2912	2917	rVB	240	176	0.02%	0.002%
68	10.679	2917	2920	2923	rBV	239	223	0.02%	0.003%
69	10.749	2927	2942	2967	rBV	251523	416669	43.03%	5.641%
70	10.856	2972	2975	2979	rVB3	321	297	0.03%	0.004%
71	10.884	2979	2984	2986	rBV2	404	351	0.04%	0.005%
72	10.955	3003	3006	3010	rBV	234	182	0.02%	0.002%
73	11.087	3041	3047	3052	rBV2	757	934	0.10%	0.013%
74	11.110	3052	3054	3056	rBV2	297	179	0.02%	0.002%
75	11.286	3102	3109	3115	rBV2	261	448	0.05%	0.006%
76	11.402	3140	3145	3147	rBV	342	251	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057890.D
 Acq On : 20 Feb 2024 10:03
 Operator : MD/SY
 Sample : VU0220WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK041

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

77	11.470	3160	3166	3174	rVB3	814	1184	0.12%	0.016%
78	11.743	3246	3251	3259	rBV6	1176	1608	0.17%	0.022%
79	11.807	3259	3271	3297	rBV	458806	751464	77.61%	10.173%
80	11.994	3324	3329	3333	rBV3	319	279	0.03%	0.004%
81	12.187	3377	3389	3418	rBV	371335	625656	64.62%	8.470%
82	12.319	3427	3430	3433	rVB	376	239	0.02%	0.003%
83	12.341	3434	3437	3441	rVB3	269	228	0.02%	0.003%
84	12.392	3448	3453	3456	rBV2	298	328	0.03%	0.004%
85	12.524	3492	3494	3499	rVB2	289	213	0.02%	0.003%
86	12.669	3535	3539	3542	rBV2	204	185	0.02%	0.003%
87	12.727	3550	3557	3560	rBV2	235	321	0.03%	0.004%
88	12.765	3564	3569	3573	rBV3	556	619	0.06%	0.008%
89	13.093	3668	3671	3673	rBV	279	232	0.02%	0.003%
90	13.187	3696	3700	3703	rBV	297	243	0.03%	0.003%
91	13.232	3708	3714	3718	rBV6	1172	1504	0.16%	0.020%
92	13.415	3767	3771	3773	rBV	243	176	0.02%	0.002%
93	13.457	3779	3784	3787	rVB2	245	237	0.02%	0.003%
94	13.576	3817	3821	3824	rBV2	260	179	0.02%	0.002%
95	13.849	3898	3906	3920	rBV2	3229	4994	0.52%	0.068%
96	14.100	3974	3984	3994	rBV2	3541	6687	0.69%	0.091%
97	14.203	4012	4016	4018	rBV2	257	253	0.03%	0.003%
98	14.334	4042	4057	4067	rBV6	3519	6464	0.67%	0.088%
99	14.537	4118	4120	4124	rBV2	295	196	0.02%	0.003%
100	14.830	4207	4211	4216	rBV3	552	697	0.07%	0.009%




Sum of corrected areas: 7386670

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057890.D
Acq On : 20 Feb 2024 10:03
Operator : MD/SY
Sample : VU0220WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK041

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

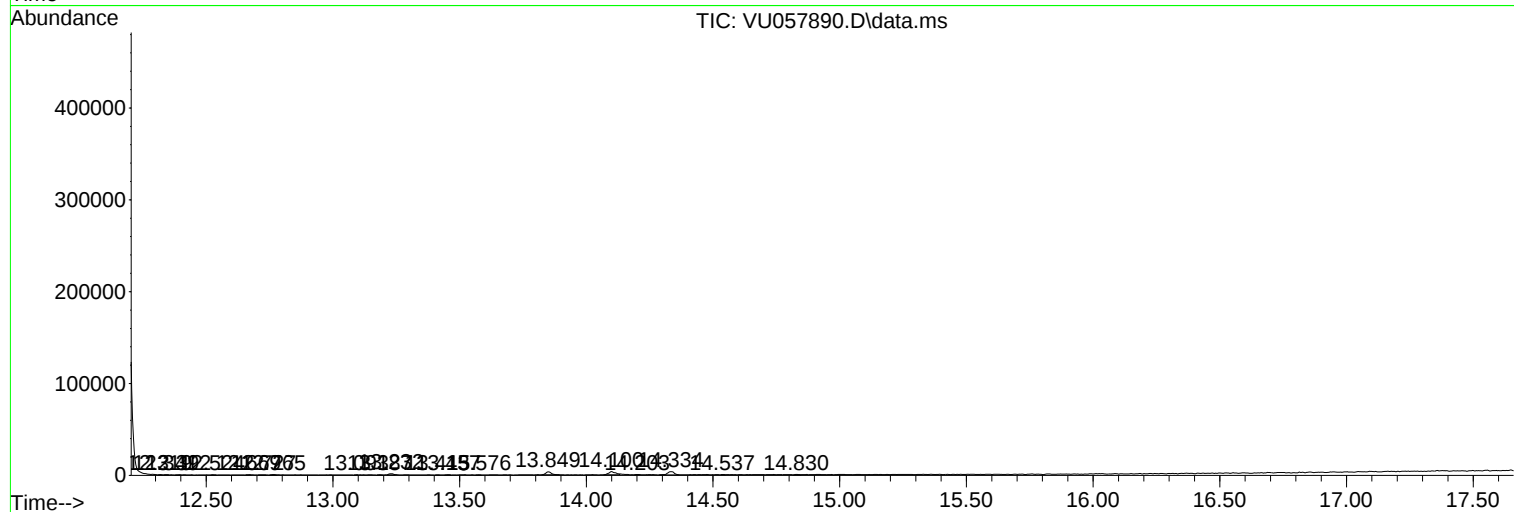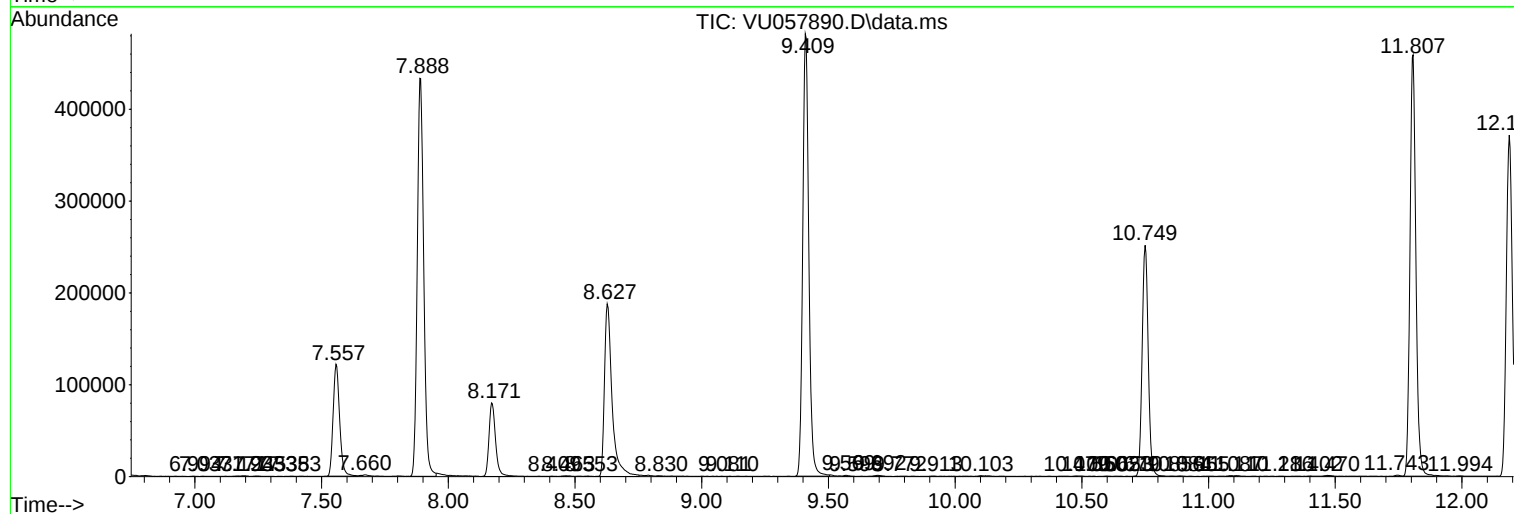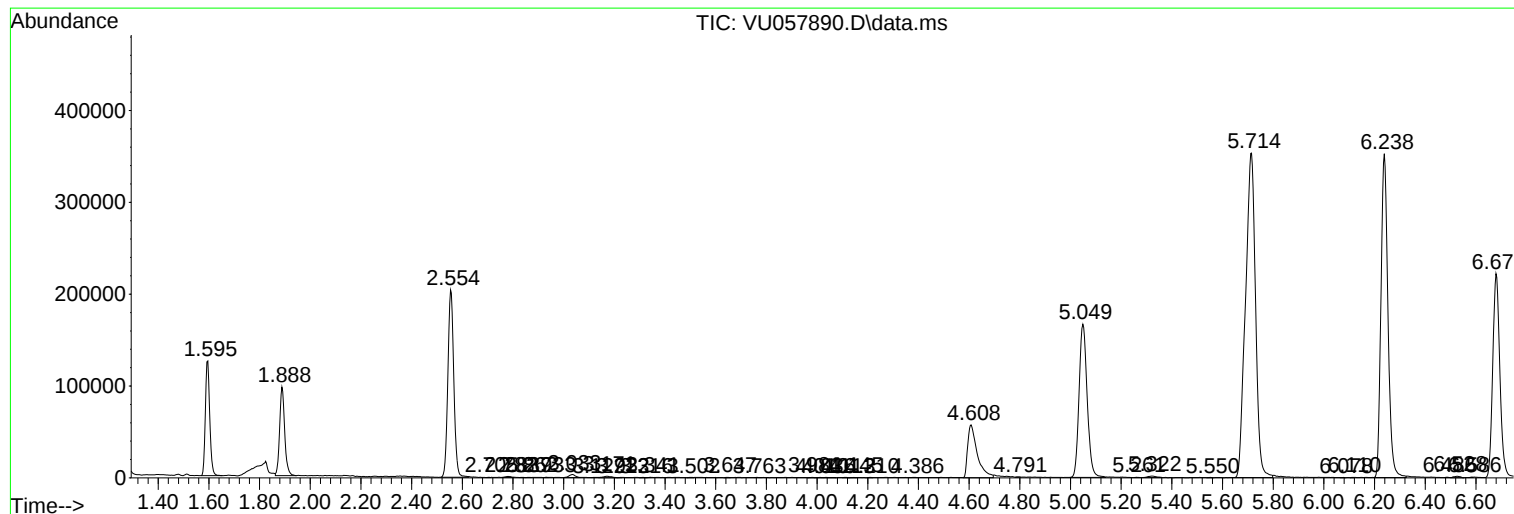

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057890.D
Acq On : 20 Feb 2024 10:03
Operator : MD/SY
Sample : VU0220WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK041

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057890.D
Acq On : 20 Feb 2024 10:03
Operator : MD/SY
Sample : VU0220WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK041

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
