

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057892.D
 Acq On : 20 Feb 2024 11:05
 Operator : MD/SY
 Sample : P1496-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHA03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

Signal : TIC: VU057892.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	111	rVB	130381	150954	15.83%	1.923%
2	1.679	114	121	133	rBV	10703	13443	1.41%	0.171%
3	1.894	180	188	209	rVB	95359	131004	13.73%	1.669%
4	2.316	317	319	322	rVB2	564	286	0.03%	0.004%
5	2.557	382	394	407	rBV	203482	330548	34.65%	4.212%
6	2.779	459	463	470	rVB3	668	890	0.09%	0.011%
7	3.033	535	542	552	rVB3	2402	4154	0.44%	0.053%
8	3.084	556	558	563	rVB2	279	203	0.02%	0.003%
9	3.171	574	585	598	rBV2	2417	6051	0.63%	0.077%
10	3.354	637	642	645	rVB3	268	240	0.03%	0.003%
11	3.457	669	674	676	rVV2	176	181	0.02%	0.002%
12	3.644	729	732	735	rVB2	305	196	0.02%	0.002%
13	3.673	735	741	743	rBV	210	202	0.02%	0.003%
14	3.846	792	795	802	rBV	284	400	0.04%	0.005%
15	4.113	872	878	884	rVB2	212	309	0.03%	0.004%
16	4.428	973	976	982	rVB2	305	334	0.04%	0.004%
17	4.470	982	989	994	rBV2	314	482	0.05%	0.006%
18	4.608	1022	1032	1071	rBV	67762	181560	19.03%	2.313%
19	4.914	1125	1127	1132	rVB2	305	223	0.02%	0.003%
20	5.052	1154	1170	1194	rBV	162276	364546	38.22%	4.645%
21	5.319	1245	1253	1256	rBV3	1222	1719	0.18%	0.022%
22	5.505	1308	1311	1316	rVB2	249	288	0.03%	0.004%
23	5.640	1349	1353	1356	rBV2	203	204	0.02%	0.003%
24	5.714	1356	1376	1402	rBV2	354609	953889	100.00%	12.154%
25	6.126	1497	1504	1510	rVB3	309	450	0.05%	0.006%
26	6.187	1514	1523	1526	rBV2	267	337	0.04%	0.004%
27	6.238	1526	1539	1562	rBV	358782	685254	71.84%	8.731%
28	6.537	1621	1632	1656	rBV5	32823	87840	9.21%	1.119%
29	6.682	1664	1677	1697	rVB	215533	422696	44.31%	5.386%
30	7.016	1775	1781	1784	rBV2	300	367	0.04%	0.005%
31	7.042	1786	1789	1797	rVB4	469	486	0.05%	0.006%
32	7.081	1797	1801	1805	rBV2	303	287	0.03%	0.004%
33	7.164	1823	1827	1831	rBV	446	412	0.04%	0.005%
34	7.200	1831	1838	1843	rVB4	1012	1274	0.13%	0.016%
35	7.389	1893	1897	1905	rBV2	153	194	0.02%	0.002%
36	7.557	1937	1949	1977	rVV	121288	221776	23.25%	2.826%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057892.D
 Acq On : 20 Feb 2024 11:05
 Operator : MD/SY
 Sample : P1496-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHA03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

37	7.705	1992	1995	1998	rBV3	376	253	0.03%	0.003%
38	7.740	2003	2006	2012	rVB3	346	351	0.04%	0.004%
39	7.791	2012	2022	2024	rBV5	2120	2576	0.27%	0.033%
40	7.891	2040	2053	2072	rBV	441135	767046	80.41%	9.774%
41	8.129	2124	2127	2130	rVB2	294	186	0.02%	0.002%
42	8.174	2130	2141	2162	rBV	82239	143843	15.08%	1.833%
43	8.306	2179	2182	2185	rBV2	398	330	0.03%	0.004%
44	8.396	2207	2210	2213	rVB2	436	307	0.03%	0.004%
45	8.418	2213	2217	2219	rBV2	263	260	0.03%	0.003%
46	8.457	2224	2229	2230	rBV3	493	424	0.04%	0.005%
47	8.505	2240	2244	2246	rBV3	241	180	0.02%	0.002%
48	8.553	2255	2259	2263	rVB3	848	804	0.08%	0.010%
49	8.627	2268	2282	2319	rBV2	220517	451762	47.36%	5.756%
50	8.914	2367	2371	2372	rBV	440	316	0.03%	0.004%
51	8.975	2387	2390	2392	rBV2	340	215	0.02%	0.003%
52	9.055	2406	2415	2420	rBV2	257	442	0.05%	0.006%
53	9.129	2432	2438	2444	rVB2	291	319	0.03%	0.004%
54	9.164	2444	2449	2454	rBV	383	462	0.05%	0.006%
55	9.286	2484	2487	2491	rVB2	252	215	0.02%	0.003%
56	9.409	2513	2525	2551	rBV	497831	839683	88.03%	10.699%
57	9.634	2590	2595	2599	rVB2	314	292	0.03%	0.004%
58	9.698	2605	2615	2624	rBV4	2125	3900	0.41%	0.050%
59	9.791	2638	2644	2646	rBV2	209	236	0.02%	0.003%
60	10.042	2719	2722	2725	rBV2	267	191	0.02%	0.002%
61	10.068	2725	2730	2732	rVV2	230	217	0.02%	0.003%
62	10.116	2732	2745	2756	rVV7	4270	10243	1.07%	0.131%
63	10.296	2798	2801	2806	rBV2	291	276	0.03%	0.004%
64	10.354	2809	2819	2828	rBV5	3048	4592	0.48%	0.059%
65	10.534	2866	2875	2877	rBV	243	242	0.03%	0.003%
66	10.749	2930	2942	2957	rBV	267752	438562	45.98%	5.588%
67	10.888	2977	2985	2993	rBV2	884	1179	0.12%	0.015%
68	11.087	3040	3047	3052	rBV3	2140	2980	0.31%	0.038%
69	11.257	3097	3100	3106	rBV2	226	255	0.03%	0.003%
70	11.466	3158	3165	3175	rBV3	3543	5051	0.53%	0.064%
71	11.560	3187	3194	3196	rBV2	251	330	0.03%	0.004%
72	11.679	3227	3231	3233	rBV2	317	210	0.02%	0.003%
73	11.714	3239	3242	3245	rBV	254	218	0.02%	0.003%
74	11.743	3246	3251	3253	rBV3	735	619	0.06%	0.008%
75	11.807	3258	3271	3293	rBV	495359	824442	86.43%	10.505%
76	12.077	3346	3355	3375	rBV5	2362	7235	0.76%	0.092%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057892.D
Acq On : 20 Feb 2024 11:05
Operator : MD/SY
Sample : P1496-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHA03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Title : VOC Analysis

77	12.187	3377	3389	3412	rBV	399327	674661	70.73%	8.596%
78	12.376	3443	3448	3453	rVB3	457	491	0.05%	0.006%
79	12.499	3481	3486	3489	rVB	351	346	0.04%	0.004%
80	12.772	3561	3571	3578	rBV3	755	1224	0.13%	0.016%
81	12.917	3614	3616	3621	rVB2	416	203	0.02%	0.003%
82	12.991	3634	3639	3653	rVB4	1756	3282	0.34%	0.042%
83	13.228	3708	3713	3719	rVB3	843	895	0.09%	0.011%
84	13.257	3719	3722	3725	rBV	288	225	0.02%	0.003%
85	13.299	3731	3735	3736	rBV	249	185	0.02%	0.002%
86	13.328	3740	3744	3746	rBV2	212	179	0.02%	0.002%
87	13.376	3754	3759	3761	rBV	329	269	0.03%	0.003%
88	13.479	3787	3791	3794	rBV	193	188	0.02%	0.002%
89	13.794	3885	3889	3891	rBV2	254	198	0.02%	0.003%
90	13.839	3894	3903	3915	rBV3	22041	34549	3.62%	0.440%
91	14.013	3950	3957	3965	rVB4	11279	15110	1.58%	0.193%
92	14.090	3969	3981	3998	rBV	18623	37197	3.90%	0.474%
93	14.293	4040	4044	4046	rBV	241	236	0.02%	0.003%
94	14.328	4051	4055	4065	rVV4	1595	2050	0.21%	0.026%
95	14.380	4069	4071	4074	rBV2	259	215	0.02%	0.003%
96	14.489	4101	4105	4107	rBV2	269	246	0.03%	0.003%
97	14.550	4121	4124	4131	rBV2	315	349	0.04%	0.004%
98	15.023	4268	4271	4275	rBV3	292	315	0.03%	0.004%
99	15.283	4348	4352	4355	rBV3	388	376	0.04%	0.005%
100	15.498	4417	4419	4421	rBV	357	214	0.02%	0.003%




Sum of corrected areas: 7848126

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057892.D
Acq On : 20 Feb 2024 11:05
Operator : MD/SY
Sample : P1496-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHA03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

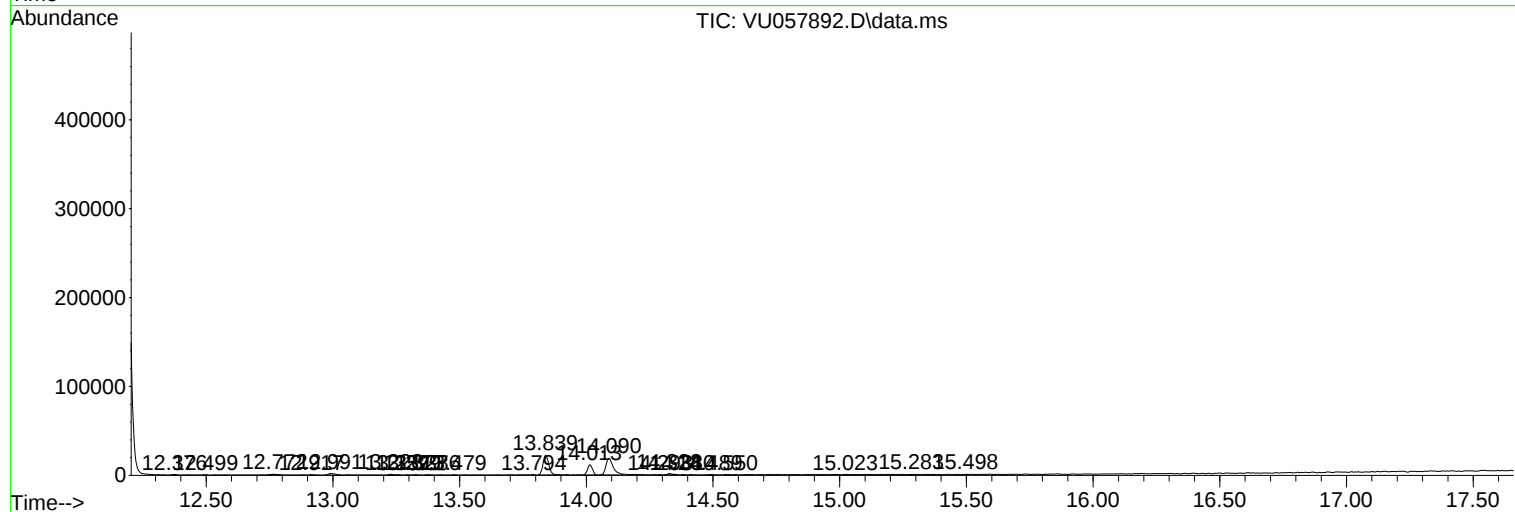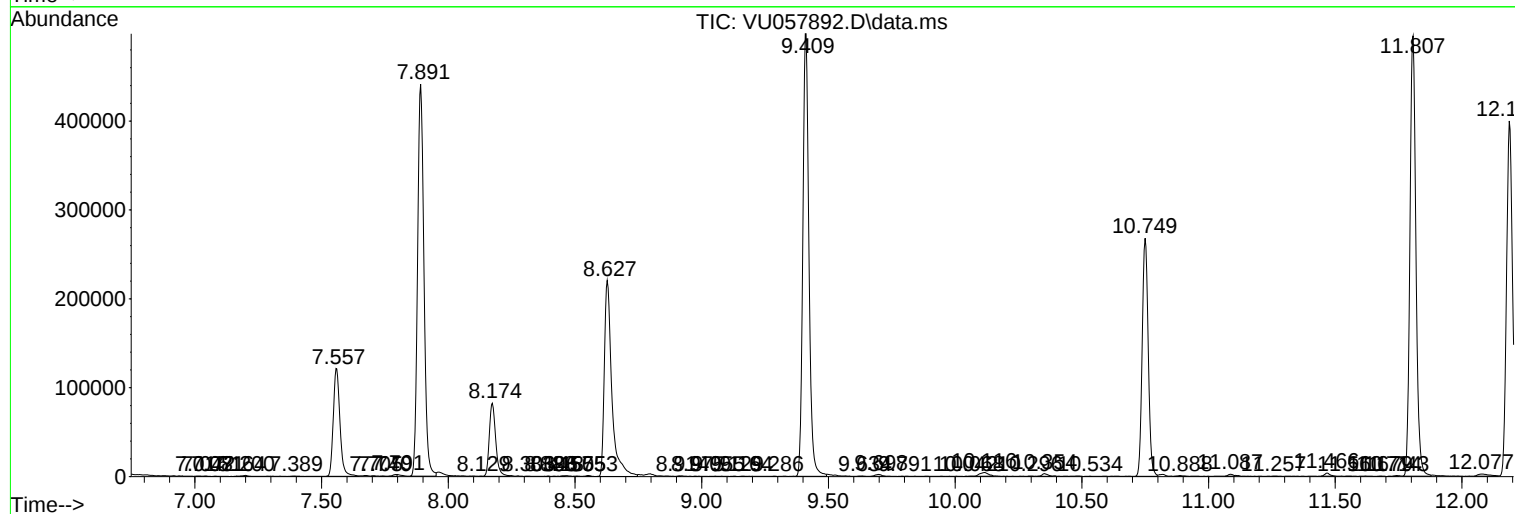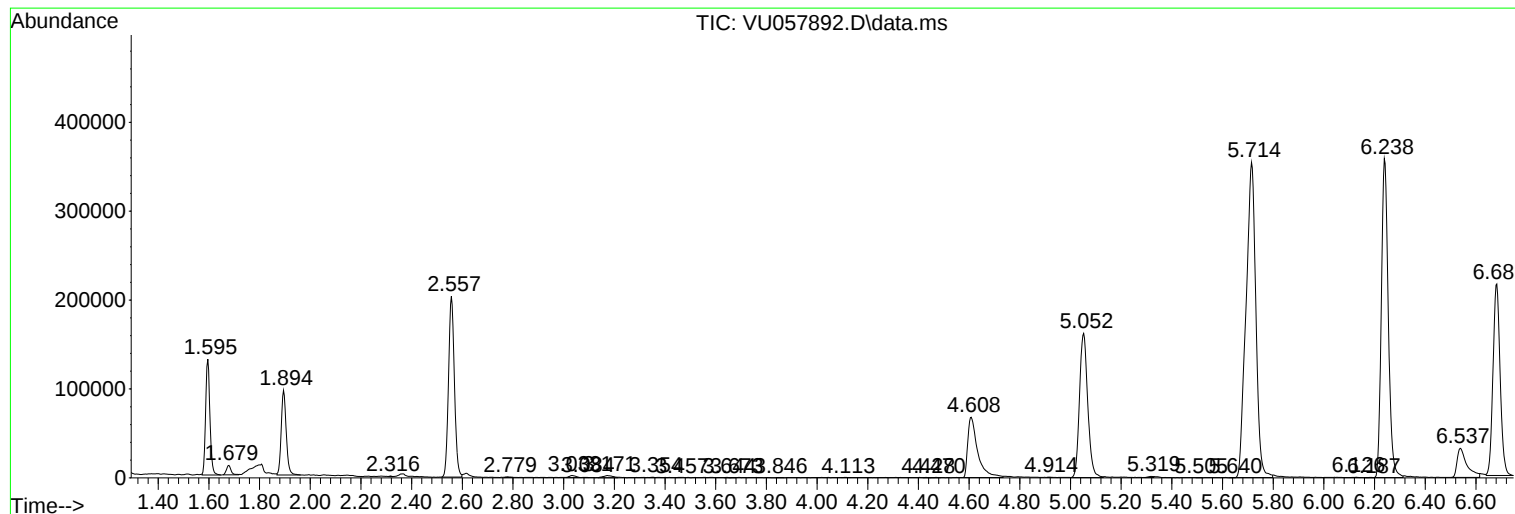

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057892.D
Acq On : 20 Feb 2024 11:05
Operator : MD/SY
Sample : P1496-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHA03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057892.D
Acq On : 20 Feb 2024 11:05
Operator : MD/SY
Sample : P1496-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHA03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------