

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057901.D
 Acq On : 20 Feb 2024 14:42
 Operator : MD/SY
 Sample : P1504-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCNB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

Signal : TIC: VU057901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	111	rVB	118172	138925	10.60%	1.556%
2	1.898	181	189	205	rVB	98662	132863	10.14%	1.488%
3	2.557	382	394	410	rBV	183530	305012	23.27%	3.416%
4	2.788	457	466	475	rVB2	909	1596	0.12%	0.018%
5	3.004	525	533	534	rBV	303	334	0.03%	0.004%
6	3.033	534	542	553	rVB3	2287	4161	0.32%	0.047%
7	3.165	576	583	586	rBV3	1196	1560	0.12%	0.017%
8	3.293	619	623	625	rBV2	198	193	0.01%	0.002%
9	3.309	625	628	629	rVV	474	291	0.02%	0.003%
10	3.348	629	640	662	rVB3	19882	44315	3.38%	0.496%
11	3.753	760	766	772	rVB2	176	252	0.02%	0.003%
12	3.798	778	780	789	rBV2	202	286	0.02%	0.003%
13	3.859	789	799	812	rBV3	1417	3055	0.23%	0.034%
14	4.412	964	971	972	rBV2	648	588	0.04%	0.007%
15	4.428	973	976	987	rVB5	993	1554	0.12%	0.017%
16	4.653	1019	1046	1082	rBV2	500841	1310627	100.00%	14.677%
17	5.049	1154	1169	1192	rBV	171313	385490	29.41%	4.317%
18	5.251	1229	1232	1236	rBV2	263	174	0.01%	0.002%
19	5.309	1244	1250	1251	rBV	666	492	0.04%	0.006%
20	5.714	1356	1376	1408	rVV2	367431	1009351	77.01%	11.303%
21	6.071	1485	1487	1490	rVB	272	173	0.01%	0.002%
22	6.123	1498	1503	1505	rVB	293	260	0.02%	0.003%
23	6.238	1525	1539	1565	rBV	377690	717460	54.74%	8.034%
24	6.499	1606	1620	1633	rVB4	4307	9871	0.75%	0.111%
25	6.679	1662	1676	1706	rBV	228548	452987	34.56%	5.073%
26	6.791	1708	1711	1712	rBV3	866	524	0.04%	0.006%
27	6.836	1722	1725	1729	rBV3	271	239	0.02%	0.003%
28	6.878	1735	1738	1741	rVB2	241	176	0.01%	0.002%
29	7.026	1780	1784	1790	rBV	138	169	0.01%	0.002%
30	7.193	1832	1836	1837	rBV2	599	366	0.03%	0.004%
31	7.296	1865	1868	1871	rVB2	264	175	0.01%	0.002%
32	7.319	1871	1875	1878	rBV	208	207	0.02%	0.002%
33	7.557	1937	1949	1969	rBV	127141	228753	17.45%	2.562%
34	7.701	1991	1994	1996	rBV2	374	259	0.02%	0.003%
35	7.737	2002	2005	2010	rVB3	300	287	0.02%	0.003%
36	7.891	2039	2053	2093	rBV	452854	796119	60.74%	8.915%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057901.D
 Acq On : 20 Feb 2024 14:42
 Operator : MD/SY
 Sample : P1504-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCNB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

37	8.171	2127	2140	2158	rBV	83620	144717	11.04%	1.621%
38	8.299	2176	2180	2184	rVB2	418	330	0.03%	0.004%
39	8.348	2192	2195	2198	rBV2	390	357	0.03%	0.004%
40	8.415	2208	2216	2223	rBV4	910	1497	0.11%	0.017%
41	8.483	2223	2237	2253	rBV3	7680	13922	1.06%	0.156%
42	8.624	2269	2281	2317	rBV2	201435	407308	31.08%	4.561%
43	8.865	2353	2356	2358	rVV2	284	186	0.01%	0.002%
44	8.907	2367	2369	2373	rVV3	250	193	0.01%	0.002%
45	9.055	2412	2415	2421	rVB2	195	196	0.01%	0.002%
46	9.148	2438	2444	2447	rBV2	183	183	0.01%	0.002%
47	9.338	2497	2503	2513	rBV3	1160	1507	0.11%	0.017%
48	9.409	2513	2525	2564	rBV	520040	879202	67.08%	9.846%
49	9.563	2571	2573	2578	rVB2	362	248	0.02%	0.003%
50	9.627	2588	2593	2597	rVB2	284	284	0.02%	0.003%
51	9.695	2607	2614	2618	rBV3	390	606	0.05%	0.007%
52	9.762	2624	2635	2647	rBV3	10871	21482	1.64%	0.241%
53	9.872	2664	2669	2672	rVB2	275	258	0.02%	0.003%
54	9.942	2685	2691	2692	rBV	198	233	0.02%	0.003%
55	10.061	2723	2728	2732	rVB	205	233	0.02%	0.003%
56	10.142	2750	2753	2759	rVB2	169	194	0.01%	0.002%
57	10.187	2762	2767	2773	rBV2	192	273	0.02%	0.003%
58	10.219	2774	2777	2781	rVB	315	217	0.02%	0.002%
59	10.251	2781	2787	2790	rBV2	232	290	0.02%	0.003%
60	10.393	2827	2831	2838	rVB2	243	253	0.02%	0.003%
61	10.512	2864	2868	2873	rVB2	179	197	0.02%	0.002%
62	10.537	2873	2876	2881	rBV2	242	178	0.01%	0.002%
63	10.592	2891	2893	2898	rBV2	279	255	0.02%	0.003%
64	10.621	2898	2902	2908	rBV2	200	277	0.02%	0.003%
65	10.750	2928	2942	2964	rBV	265724	430531	32.85%	4.821%
66	10.881	2980	2983	2991	rVB2	326	372	0.03%	0.004%
67	11.061	3034	3039	3044	rBV2	228	278	0.02%	0.003%
68	11.402	3141	3145	3146	rBV2	556	373	0.03%	0.004%
69	11.479	3165	3169	3174	rBV	366	317	0.02%	0.004%
70	11.502	3174	3176	3179	rVB2	287	178	0.01%	0.002%
71	11.611	3206	3210	3214	rBV	297	317	0.02%	0.004%
72	11.643	3214	3220	3224	rBV3	1006	1181	0.09%	0.013%
73	11.692	3230	3235	3238	rBV	164	175	0.01%	0.002%
74	11.804	3258	3270	3295	rBV	497901	810710	61.86%	9.079%
75	12.074	3348	3354	3355	rBV2	512	427	0.03%	0.005%
76	12.187	3376	3389	3419	rBV	396503	653588	49.87%	7.319%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057901.D
 Acq On : 20 Feb 2024 14:42
 Operator : MD/SY
 Sample : P1504-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCNB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

77	12.322	3427	3431	3433	rBV	237	216	0.02%	0.002%
78	12.386	3448	3451	3455	rVB	340	235	0.02%	0.003%
79	12.473	3474	3478	3481	rBV	375	302	0.02%	0.003%
80	12.733	3554	3559	3563	rVV2	294	351	0.03%	0.004%
81	12.766	3564	3569	3578	rVV3	634	780	0.06%	0.009%
82	12.817	3582	3585	3594	rVB2	216	291	0.02%	0.003%
83	12.856	3594	3597	3602	rBV2	372	373	0.03%	0.004%
84	13.235	3712	3715	3720	rVB2	201	209	0.02%	0.002%
85	13.264	3720	3724	3728	rBV	286	246	0.02%	0.003%
86	13.643	3838	3842	3844	rBV2	211	168	0.01%	0.002%
87	13.791	3885	3888	3890	rBV	213	169	0.01%	0.002%
88	13.843	3900	3904	3907	rBV2	298	308	0.02%	0.003%
89	13.917	3924	3927	3932	rVB2	239	186	0.01%	0.002%
90	14.174	4002	4007	4010	rVB2	285	262	0.02%	0.003%
91	14.280	4035	4040	4042	rBV2	397	309	0.02%	0.003%
92	14.730	4177	4180	4182	rBV3	208	169	0.01%	0.002%
93	14.833	4209	4212	4214	rBV2	332	235	0.02%	0.003%
94	15.254	4341	4343	4348	rBV2	251	226	0.02%	0.003%
95	15.299	4355	4357	4362	rVB2	324	224	0.02%	0.003%
96	15.341	4368	4370	4372	rBV2	328	184	0.01%	0.002%
97	15.386	4381	4384	4386	rBV3	307	219	0.02%	0.002%
98	15.418	4392	4394	4396	rBV	340	241	0.02%	0.003%
99	15.688	4475	4478	4481	rBV2	441	335	0.03%	0.004%
100	16.495	4725	4729	4732	rBV4	953	909	0.07%	0.010%




Sum of corrected areas: 8929814

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057901.D
Acq On : 20 Feb 2024 14:42
Operator : MD/SY
Sample : P1504-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCNB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

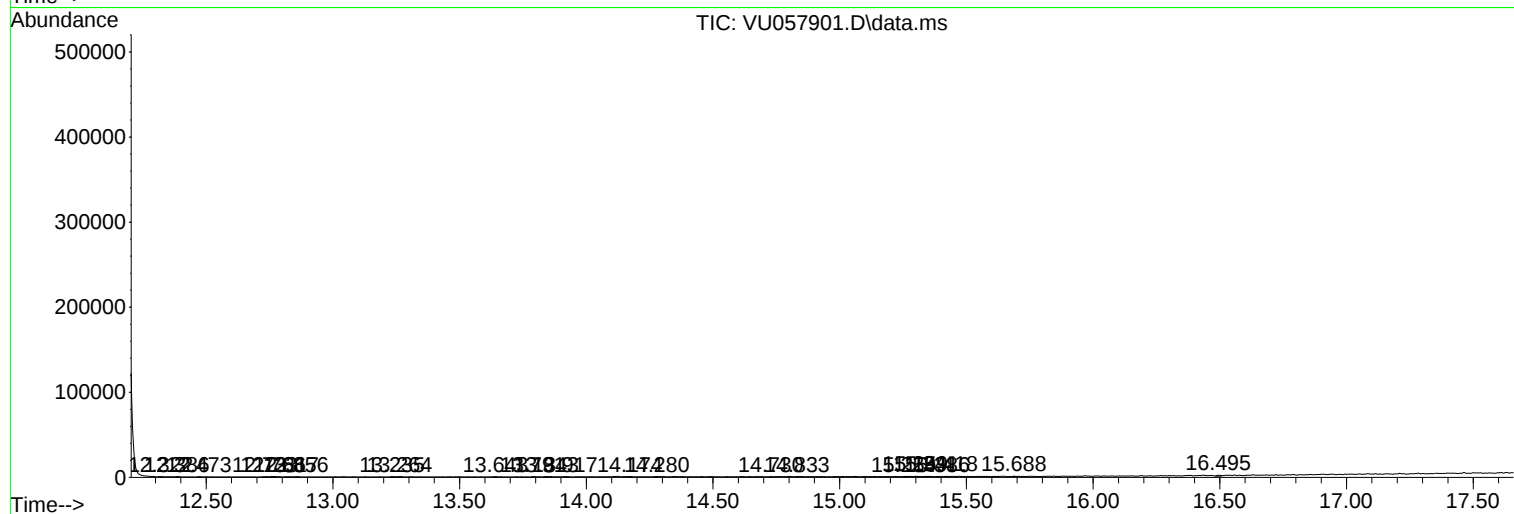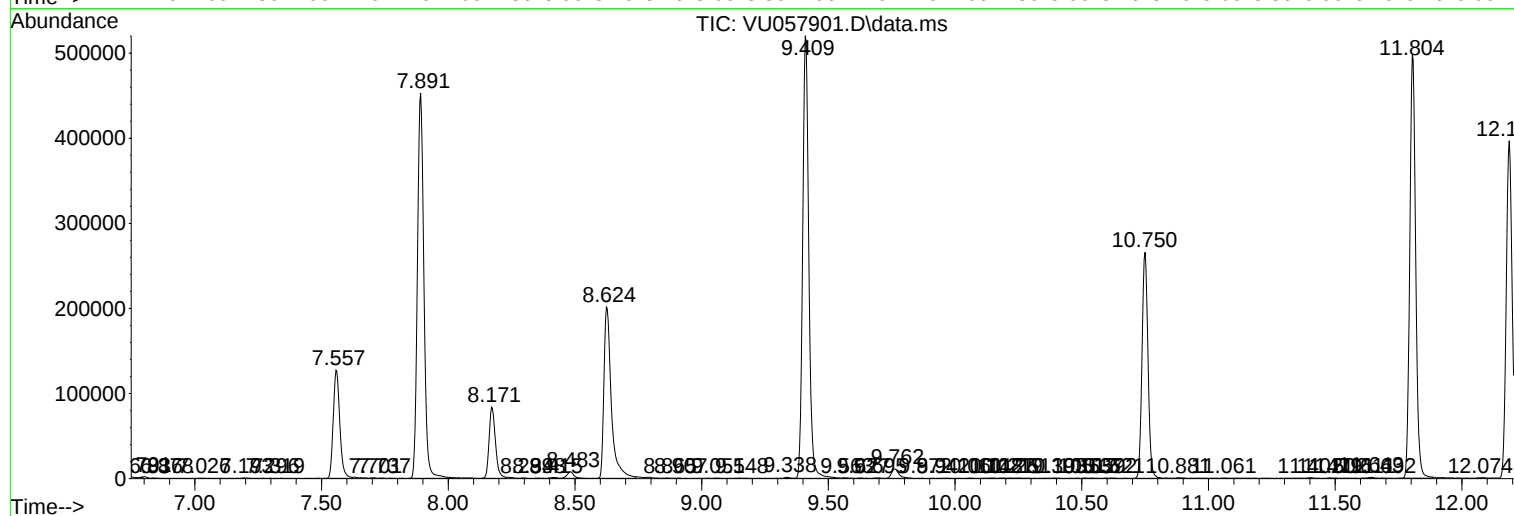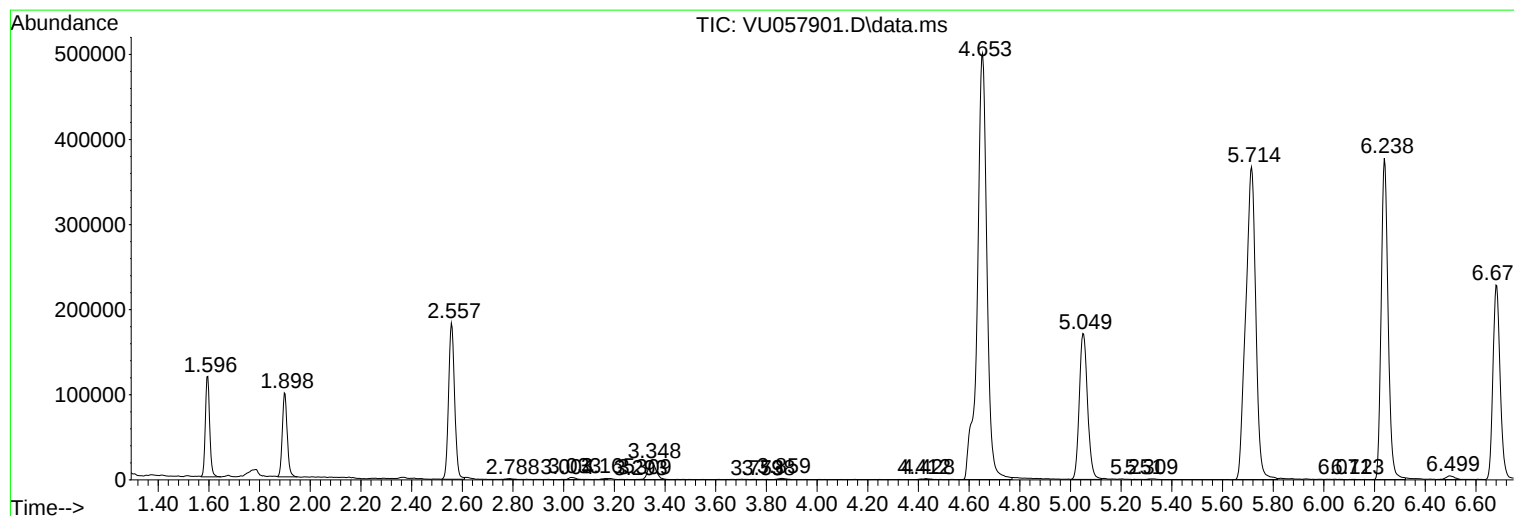

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057901.D
Acq On : 20 Feb 2024 14:42
Operator : MD/SY
Sample : P1504-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCNB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057901.D
Acq On : 20 Feb 2024 14:42
Operator : MD/SY
Sample : P1504-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCNB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------