

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057903.D
 Acq On : 20 Feb 2024 15:30
 Operator : MD/SY
 Sample : P1504-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCNE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

Signal : TIC: VU057903.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	113	rVB	141188	165232	5.74%	1.502%
2	1.907	184	192	207	rVB	103172	137581	4.78%	1.251%
3	2.560	382	395	413	rBV	212296	356421	12.38%	3.240%
4	2.698	435	438	443	rVB	299	194	0.01%	0.002%
5	2.769	458	460	461	rVV	514	265	0.01%	0.002%
6	2.788	461	466	476	rVB3	1621	2592	0.09%	0.024%
7	2.923	506	508	511	rVB3	406	223	0.01%	0.002%
8	2.952	511	517	518	rBV2	394	412	0.01%	0.004%
9	3.039	535	544	551	rBV3	1929	2990	0.10%	0.027%
10	3.171	578	585	595	rVB2	872	1886	0.07%	0.017%
11	3.345	625	639	669	rBV	273260	549107	19.08%	4.992%
12	3.820	783	787	790	rBV	241	239	0.01%	0.002%
13	3.862	792	800	811	rVB3	811	1819	0.06%	0.017%
14	4.135	882	885	889	rVB	225	179	0.01%	0.002%
15	4.158	889	892	894	rBV	232	188	0.01%	0.002%
16	4.303	934	937	942	rBV2	194	228	0.01%	0.002%
17	4.653	1022	1046	1086	rBV	1187235	2878267	100.00%	26.167%
18	5.052	1155	1170	1197	rBV	173226	384072	13.34%	3.492%
19	5.293	1243	1245	1250	rVB3	323	237	0.01%	0.002%
20	5.316	1250	1252	1258	rVB3	401	338	0.01%	0.003%
21	5.344	1258	1261	1268	rVB2	287	248	0.01%	0.002%
22	5.640	1348	1353	1356	rBV	196	212	0.01%	0.002%
23	5.714	1356	1376	1409	rBV2	365674	1008278	35.03%	9.166%
24	5.965	1451	1454	1455	rBV	259	171	0.01%	0.002%
25	6.013	1465	1469	1474	rBV4	406	550	0.02%	0.005%
26	6.123	1502	1503	1506	rVB2	385	186	0.01%	0.002%
27	6.184	1516	1522	1524	rBV2	249	219	0.01%	0.002%
28	6.242	1526	1540	1564	rBV	360481	698012	24.25%	6.346%
29	6.502	1611	1621	1637	rVB3	3619	7432	0.26%	0.068%
30	6.682	1664	1677	1701	rBV	227368	449093	15.60%	4.083%
31	6.865	1731	1734	1737	rBV	465	283	0.01%	0.003%
32	7.077	1796	1800	1802	rBV2	200	196	0.01%	0.002%
33	7.139	1816	1819	1823	rVB	273	236	0.01%	0.002%
34	7.193	1831	1836	1837	rBV2	380	255	0.01%	0.002%
35	7.303	1866	1870	1873	rBV	190	208	0.01%	0.002%
36	7.351	1883	1885	1889	rVB2	251	160	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057903.D
 Acq On : 20 Feb 2024 15:30
 Operator : MD/SY
 Sample : P1504-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCNE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

37	7.373	1890	1892	1898	rBV2	186	171	0.01%	0.002%
38	7.405	1898	1902	1905	rBV	211	191	0.01%	0.002%
39	7.428	1906	1909	1913	rBV2	248	190	0.01%	0.002%
40	7.489	1923	1928	1937	rBV2	280	492	0.02%	0.004%
41	7.560	1937	1950	1977	rBV	125842	231277	8.04%	2.103%
42	7.711	1993	1997	2000	rBV3	385	345	0.01%	0.003%
43	7.891	2040	2053	2086	rBV	456297	803389	27.91%	7.304%
44	8.174	2130	2141	2163	rBV	81905	146823	5.10%	1.335%
45	8.357	2195	2198	2206	rVB2	259	348	0.01%	0.003%
46	8.405	2207	2213	2214	rBV2	176	174	0.01%	0.002%
47	8.450	2225	2227	2230	rBV2	282	230	0.01%	0.002%
48	8.483	2230	2237	2246	rVB6	1197	1967	0.07%	0.018%
49	8.569	2261	2264	2267	rBV2	238	173	0.01%	0.002%
50	8.624	2271	2281	2316	rBV2	193184	395423	13.74%	3.595%
51	8.865	2350	2356	2359	rBV3	327	294	0.01%	0.003%
52	9.293	2486	2489	2493	rBV2	214	204	0.01%	0.002%
53	9.412	2510	2526	2550	rBV	496212	849927	29.53%	7.727%
54	9.647	2594	2599	2602	rBV2	229	261	0.01%	0.002%
55	9.695	2611	2614	2618	rBV2	236	226	0.01%	0.002%
56	9.762	2625	2635	2650	rBV3	3393	6948	0.24%	0.063%
57	10.100	2736	2740	2747	rVB2	309	387	0.01%	0.004%
58	10.174	2759	2763	2767	rBV2	155	168	0.01%	0.002%
59	10.319	2803	2808	2811	rBV2	323	303	0.01%	0.003%
60	10.415	2833	2838	2841	rBV2	181	160	0.01%	0.001%
61	10.511	2864	2868	2872	rVB2	190	158	0.01%	0.001%
62	10.749	2929	2942	2964	rBV	257097	423827	14.73%	3.853%
63	10.881	2980	2983	2984	rBV2	255	175	0.01%	0.002%
64	10.984	3006	3015	3018	rBV2	284	463	0.02%	0.004%
65	11.161	3063	3070	3072	rBV	272	373	0.01%	0.003%
66	11.212	3082	3086	3092	rVB	199	197	0.01%	0.002%
67	11.399	3140	3144	3145	rBV	365	192	0.01%	0.002%
68	11.624	3210	3214	3216	rBV2	290	278	0.01%	0.003%
69	11.650	3218	3222	3228	rVB3	429	494	0.02%	0.004%
70	11.743	3248	3251	3254	rBV	260	233	0.01%	0.002%
71	11.804	3258	3270	3301	rBV	490441	808777	28.10%	7.353%
72	12.000	3327	3331	3333	rBV3	325	314	0.01%	0.003%
73	12.187	3375	3389	3421	rBV	397971	668744	23.23%	6.080%
74	12.437	3464	3467	3472	rVB	294	249	0.01%	0.002%
75	12.463	3472	3475	3476	rBV	268	163	0.01%	0.001%
76	12.582	3508	3512	3515	rBV	309	284	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057903.D
 Acq On : 20 Feb 2024 15:30
 Operator : MD/SY
 Sample : P1504-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCNE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

77	12.688	3543	3545	3548	rBV2	266	191	0.01%	0.002%
78	12.794	3575	3578	3581	rBB2	280	178	0.01%	0.002%
79	12.830	3586	3589	3594	rVV2	192	194	0.01%	0.002%
80	13.174	3693	3696	3700	rBV	212	157	0.01%	0.001%
81	13.505	3797	3799	3801	rVV	315	176	0.01%	0.002%
82	13.524	3802	3805	3809	rVB2	383	332	0.01%	0.003%
83	13.627	3832	3837	3841	rBV2	258	320	0.01%	0.003%
84	13.801	3889	3891	3896	rVB2	304	177	0.01%	0.002%
85	13.865	3909	3911	3914	rBV	352	229	0.01%	0.002%
86	13.926	3928	3930	3936	rVB2	283	197	0.01%	0.002%
87	14.125	3988	3992	3995	rBV2	371	364	0.01%	0.003%
88	14.460	4093	4096	4100	rBV2	197	180	0.01%	0.002%
89	14.479	4100	4102	4108	rVB2	355	311	0.01%	0.003%
90	14.646	4151	4154	4156	rBV2	408	280	0.01%	0.003%
91	14.695	4166	4169	4171	rBV2	338	229	0.01%	0.002%
92	14.759	4184	4189	4192	rBV2	333	344	0.01%	0.003%
93	14.830	4208	4211	4214	rVB2	377	227	0.01%	0.002%
94	14.852	4214	4218	4219	rBV	334	237	0.01%	0.002%
95	14.916	4234	4238	4239	rBV	469	397	0.01%	0.004%
96	15.431	4395	4398	4402	rBV3	328	254	0.01%	0.002%
97	15.466	4406	4409	4412	rVV2	502	336	0.01%	0.003%
98	15.611	4448	4454	4456	rBV4	406	398	0.01%	0.004%
99	15.688	4476	4478	4481	rBV	403	209	0.01%	0.002%
100	15.727	4486	4490	4492	rBV2	627	517	0.02%	0.005%




Sum of corrected areas: 10999635

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057903.D
Acq On : 20 Feb 2024 15:30
Operator : MD/SY
Sample : P1504-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCNE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

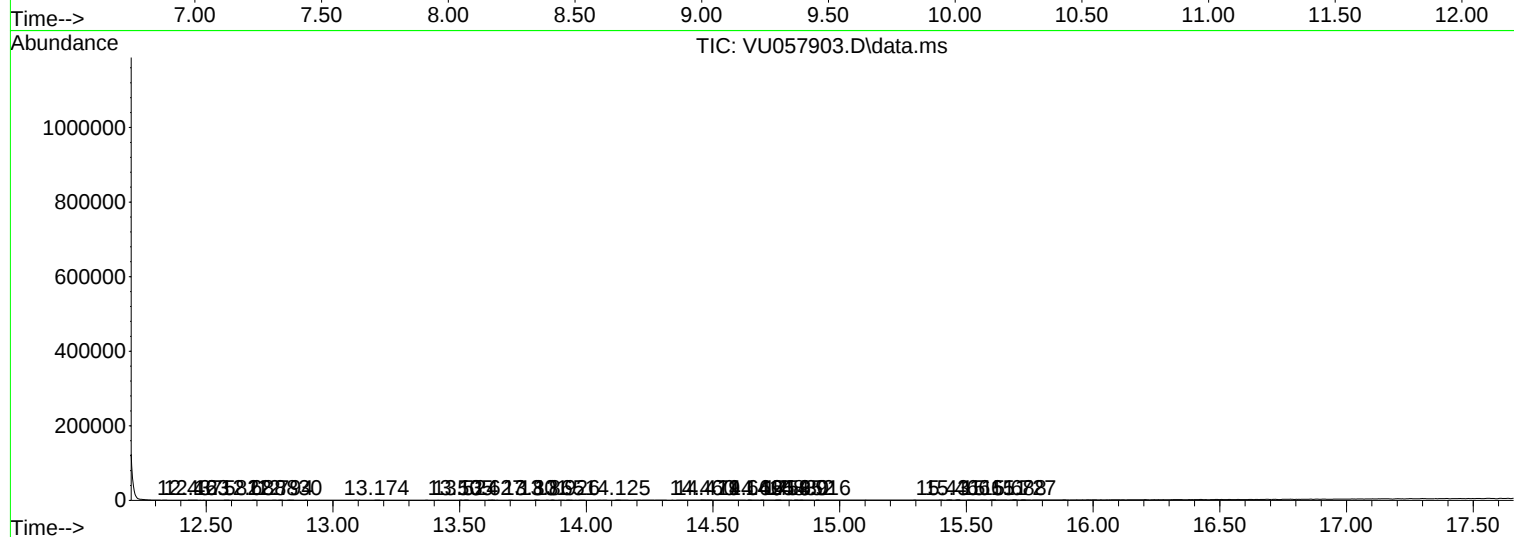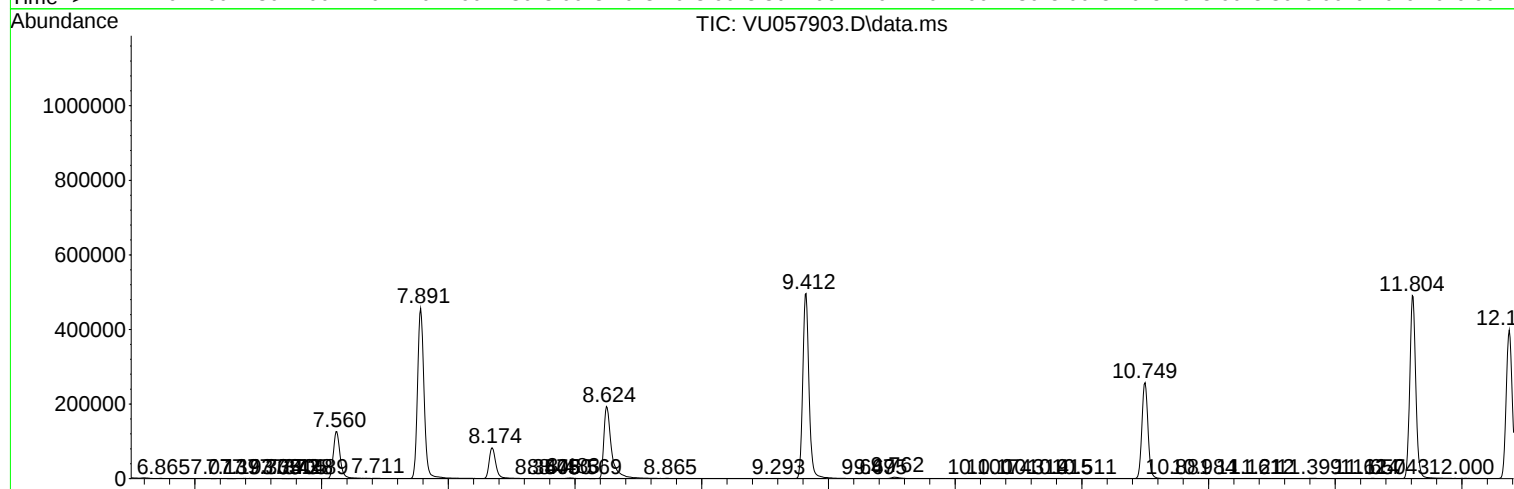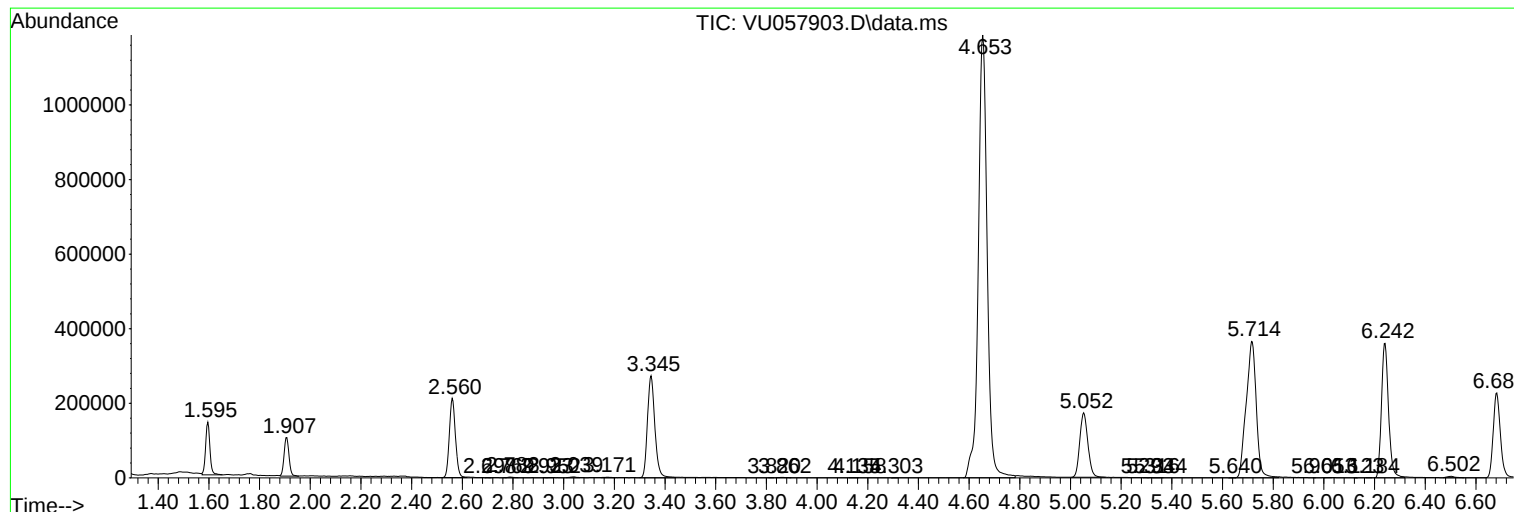

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057903.D
Acq On : 20 Feb 2024 15:30
Operator : MD/SY
Sample : P1504-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCNE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057903.D
Acq On : 20 Feb 2024 15:30
Operator : MD/SY
Sample : P1504-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCNE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc