

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057904.D
 Acq On : 20 Feb 2024 15:54
 Operator : MD/SY
 Sample : P1504-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

Signal : TIC: VU057904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	113	rVB	139731	157179	15.01%	1.929%
2	1.907	183	192	207	rBV	108489	140910	13.46%	1.729%
3	2.560	382	395	411	rBV	212637	350346	33.46%	4.300%
4	2.785	457	465	476	rVV2	2004	3291	0.31%	0.040%
5	2.991	523	529	531	rBV2	247	172	0.02%	0.002%
6	3.039	535	544	554	rVB4	2324	3799	0.36%	0.047%
7	3.168	575	584	585	rBV4	778	950	0.09%	0.012%
8	3.351	628	641	653	rBV2	4672	8928	0.85%	0.110%
9	3.586	709	714	718	rBV2	146	186	0.02%	0.002%
10	3.717	752	755	760	rVB2	202	198	0.02%	0.002%
11	3.814	780	785	788	rBV2	272	268	0.03%	0.003%
12	4.155	889	891	896	rVB2	209	160	0.02%	0.002%
13	4.274	923	928	934	rVB2	273	409	0.04%	0.005%
14	4.312	934	940	943	rBV2	280	393	0.04%	0.005%
15	4.351	947	952	955	rBV2	238	268	0.03%	0.003%
16	4.608	1017	1032	1081	rBV	64979	213361	20.37%	2.619%
17	5.052	1154	1170	1192	rBV	180823	402130	38.40%	4.935%
18	5.203	1215	1217	1223	rVB4	721	457	0.04%	0.006%
19	5.399	1274	1278	1285	rVB2	138	169	0.02%	0.002%
20	5.438	1285	1290	1293	rBV2	196	174	0.02%	0.002%
21	5.608	1339	1343	1346	rVB2	196	173	0.02%	0.002%
22	5.714	1355	1376	1400	rBV2	386503	1047215	100.00%	12.853%
23	5.939	1444	1446	1452	rVB2	473	371	0.04%	0.005%
24	6.123	1496	1503	1509	rBV3	408	511	0.05%	0.006%
25	6.241	1527	1540	1568	rBV	378937	743676	71.01%	9.127%
26	6.422	1593	1596	1599	rVB3	517	319	0.03%	0.004%
27	6.438	1599	1601	1605	rVB	277	177	0.02%	0.002%
28	6.521	1622	1627	1634	rBV5	910	1216	0.12%	0.015%
29	6.682	1661	1677	1699	rBV	239129	473422	45.21%	5.810%
30	6.849	1727	1729	1737	rVB3	594	580	0.06%	0.007%
31	6.891	1738	1742	1746	rBV	494	419	0.04%	0.005%
32	6.936	1750	1756	1759	rVB2	204	252	0.02%	0.003%
33	6.955	1759	1762	1767	rBV2	224	251	0.02%	0.003%
34	7.196	1831	1837	1839	rBV2	511	461	0.04%	0.006%
35	7.235	1845	1849	1857	rVB3	368	436	0.04%	0.005%
36	7.560	1938	1950	1969	rBV	130979	239888	22.91%	2.944%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057904.D
 Acq On : 20 Feb 2024 15:54
 Operator : MD/SY
 Sample : P1504-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

37	7.891	2040	2053	2090	rBV	475501	842647	80.47%	10.342%
38	8.174	2130	2141	2168	rVV	88861	157339	15.02%	1.931%
39	8.434	2219	2222	2226	rVV2	209	213	0.02%	0.003%
40	8.457	2226	2229	2235	rVV3	368	441	0.04%	0.005%
41	8.624	2271	2281	2325	rBV2	206760	440436	42.06%	5.406%
42	8.807	2336	2338	2345	rVB3	581	681	0.07%	0.008%
43	8.833	2345	2346	2349	rBV	303	162	0.02%	0.002%
44	8.868	2354	2357	2360	rBV	521	395	0.04%	0.005%
45	9.077	2418	2422	2427	rBV2	260	238	0.02%	0.003%
46	9.158	2441	2447	2452	rVB2	153	224	0.02%	0.003%
47	9.212	2458	2464	2467	rBV2	208	280	0.03%	0.003%
48	9.412	2512	2526	2554	rBV	522480	908367	86.74%	11.148%
49	9.621	2588	2591	2595	rBV3	240	218	0.02%	0.003%
50	9.669	2603	2606	2610	rBV	264	204	0.02%	0.003%
51	9.695	2610	2614	2621	rBV	285	278	0.03%	0.003%
52	9.775	2636	2639	2644	rVB2	265	227	0.02%	0.003%
53	9.801	2644	2647	2650	rBV2	207	168	0.02%	0.002%
54	9.971	2698	2700	2705	rVV2	197	205	0.02%	0.003%
55	10.106	2738	2742	2745	rBV	268	203	0.02%	0.002%
56	10.171	2758	2762	2767	rVB	203	199	0.02%	0.002%
57	10.254	2785	2788	2791	rBV	252	211	0.02%	0.003%
58	10.331	2809	2812	2816	rVB2	201	161	0.02%	0.002%
59	10.749	2929	2942	2963	rBV	274109	447268	42.71%	5.489%
60	10.888	2980	2985	2988	rBV2	247	338	0.03%	0.004%
61	10.904	2988	2990	2993	rVB3	428	229	0.02%	0.003%
62	10.978	3009	3013	3016	rBV	272	266	0.03%	0.003%
63	11.058	3036	3038	3042	rVV	310	214	0.02%	0.003%
64	11.460	3160	3163	3171	rBV2	206	201	0.02%	0.002%
65	11.572	3194	3198	3202	rBV2	254	307	0.03%	0.004%
66	11.708	3237	3240	3242	rBV	223	180	0.02%	0.002%
67	11.756	3251	3255	3258	rBV	312	290	0.03%	0.004%
68	11.804	3258	3270	3299	rVV	515514	851654	81.33%	10.452%
69	12.003	3328	3332	3333	rBV	338	199	0.02%	0.002%
70	12.074	3352	3354	3359	rVB	312	244	0.02%	0.003%
71	12.097	3359	3361	3365	rBV	252	176	0.02%	0.002%
72	12.187	3376	3389	3410	rBV	413854	691773	66.06%	8.490%
73	12.524	3489	3494	3497	rBV2	294	319	0.03%	0.004%
74	12.608	3517	3520	3525	rBV2	199	190	0.02%	0.002%
75	12.717	3550	3554	3559	rBV2	215	272	0.03%	0.003%
76	12.875	3598	3603	3605	rBV	286	244	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057904.D
 Acq On : 20 Feb 2024 15:54
 Operator : MD/SY
 Sample : P1504-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

77	12.942	3619	3624	3631	rBV2	336	443	0.04%	0.005%
78	12.978	3631	3635	3639	rVV2	211	223	0.02%	0.003%
79	13.039	3648	3654	3657	rBV2	266	299	0.03%	0.004%
80	13.338	3744	3747	3753	rBV2	256	288	0.03%	0.004%
81	13.688	3853	3856	3860	rBV	223	232	0.02%	0.003%
82	13.842	3900	3904	3907	rVB2	345	233	0.02%	0.003%
83	13.865	3908	3911	3916	rBV3	369	351	0.03%	0.004%
84	13.926	3925	3930	3932	rBV2	283	261	0.02%	0.003%
85	14.087	3977	3980	3981	rBV	270	168	0.02%	0.002%
86	14.119	3987	3990	3993	rVB	376	189	0.02%	0.002%
87	14.141	3993	3997	3998	rBV2	374	294	0.03%	0.004%
88	14.177	4004	4008	4010	rVB	313	211	0.02%	0.003%
89	14.267	4030	4036	4040	rBV2	288	338	0.03%	0.004%
90	14.669	4158	4161	4163	rBV	439	322	0.03%	0.004%
91	15.087	4288	4291	4294	rVB	412	249	0.02%	0.003%
92	15.106	4294	4297	4298	rBV2	345	235	0.02%	0.003%
93	15.392	4383	4386	4391	rBV3	361	444	0.04%	0.005%
94	15.437	4397	4400	4402	rBV2	255	175	0.02%	0.002%
95	15.720	4485	4488	4489	rBV	457	196	0.02%	0.002%
96	15.775	4501	4505	4508	rBV2	681	535	0.05%	0.007%
97	15.830	4520	4522	4525	rVB3	616	309	0.03%	0.004%
98	15.852	4525	4529	4530	rBV	371	292	0.03%	0.004%
99	15.971	4563	4566	4568	rBV	540	370	0.04%	0.005%
100	16.164	4624	4626	4628	rBV3	507	273	0.03%	0.003%




Sum of corrected areas: 8147906

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057904.D
Acq On : 20 Feb 2024 15:54
Operator : MD/SY
Sample : P1504-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

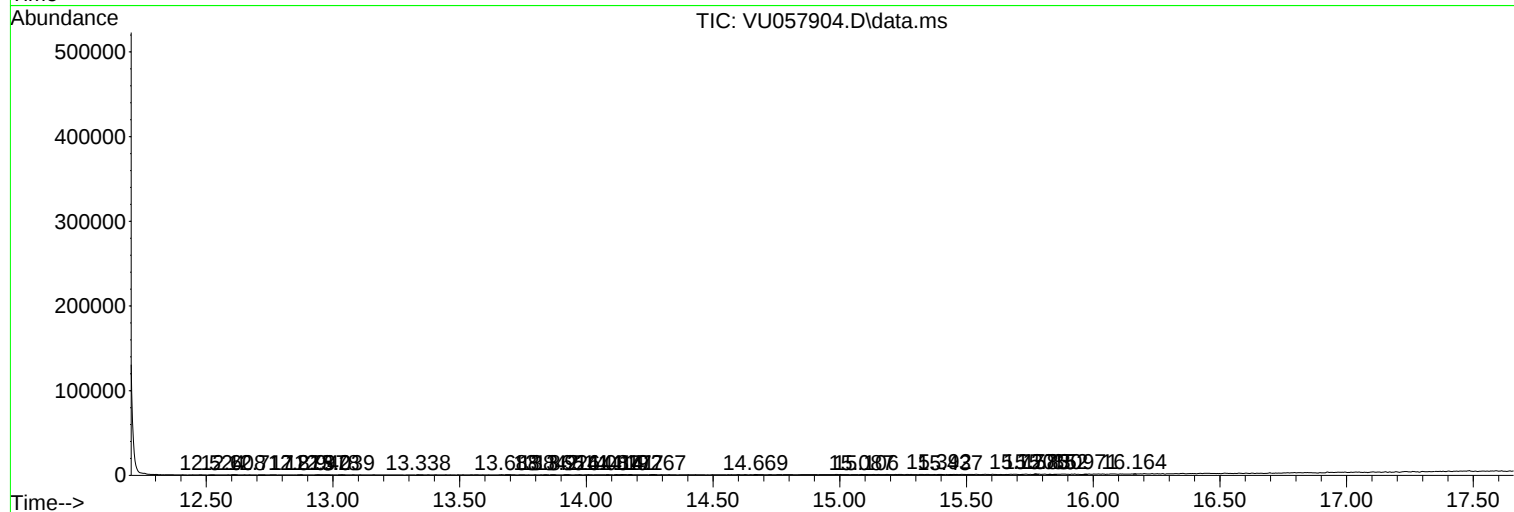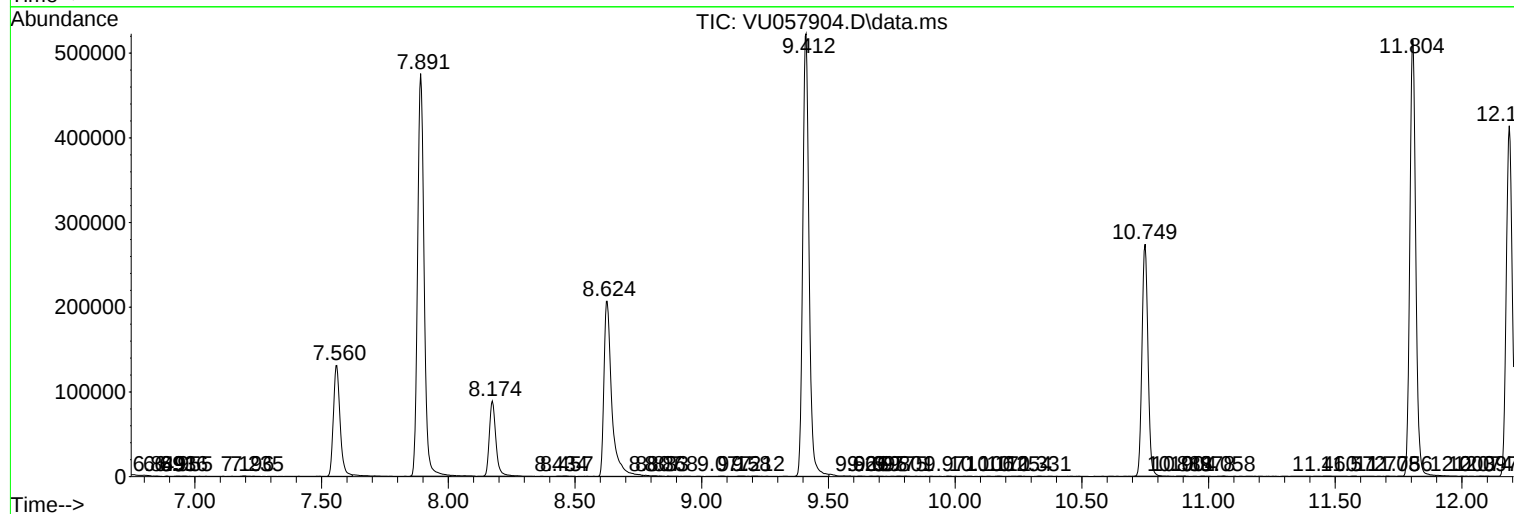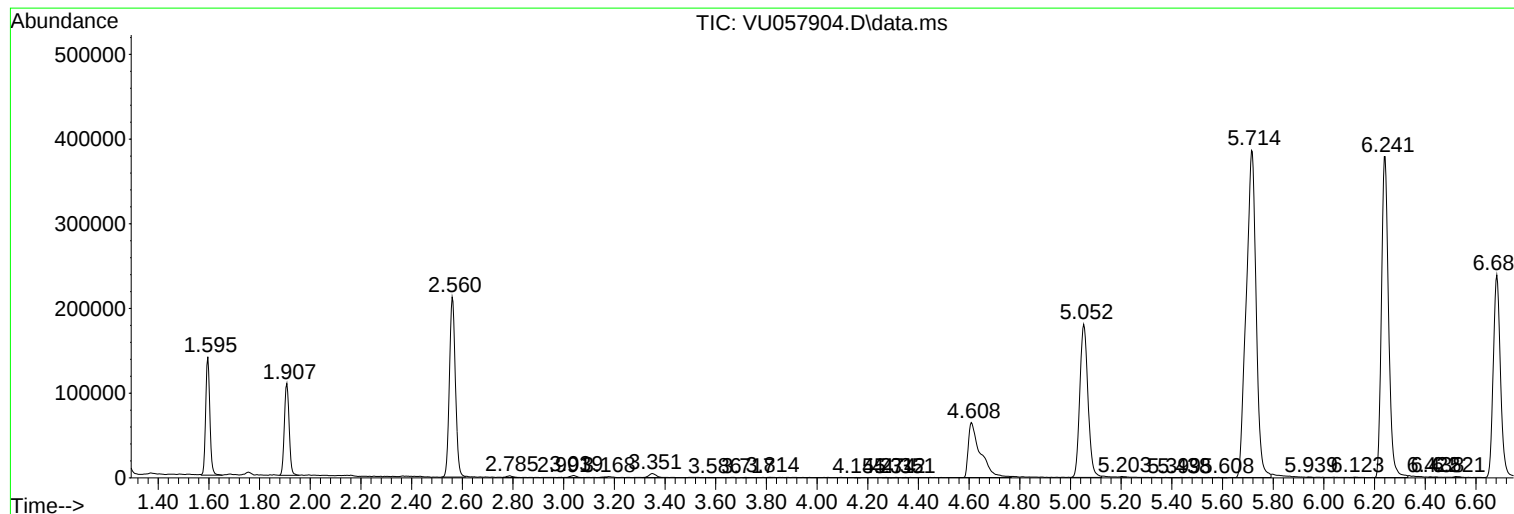

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057904.D
Acq On : 20 Feb 2024 15:54
Operator : MD/SY
Sample : P1504-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057904.D
Acq On : 20 Feb 2024 15:54
Operator : MD/SY
Sample : P1504-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------