

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057905.D
 Acq On : 20 Feb 2024 16:18
 Operator : MD/SY
 Sample : P1513-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

Signal : TIC: VU057905.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	106	rBV	134475	150754	14.71%	1.899%
2	1.907	183	192	207	rVB	106632	137917	13.46%	1.737%
3	2.560	383	395	418	rBV	209085	342912	33.47%	4.320%
4	2.721	442	445	447	rBV	221	136	0.01%	0.002%
5	2.737	447	450	453	rBV3	419	280	0.03%	0.004%
6	2.785	457	465	466	rBV3	1377	1302	0.13%	0.016%
7	2.856	483	487	490	rBV2	287	270	0.03%	0.003%
8	3.036	534	543	554	rBV4	2299	4203	0.41%	0.053%
9	3.126	565	571	576	rBV	293	371	0.04%	0.005%
10	3.171	576	585	596	rVV3	1237	2626	0.26%	0.033%
11	3.351	633	641	653	rVB6	1992	3813	0.37%	0.048%
12	3.409	653	659	663	rBV2	229	355	0.03%	0.004%
13	3.721	753	756	760	rBV2	129	136	0.01%	0.002%
14	3.843	792	794	798	rVB2	217	144	0.01%	0.002%
15	3.869	798	802	805	rBV2	201	176	0.02%	0.002%
16	4.135	878	885	887	rBV	267	371	0.04%	0.005%
17	4.335	944	947	949	rBV	174	151	0.01%	0.002%
18	4.354	949	953	959	rVV2	315	319	0.03%	0.004%
19	4.399	963	967	969	rBV	262	240	0.02%	0.003%
20	4.467	985	988	991	rBV2	205	150	0.01%	0.002%
21	4.515	996	1003	1006	rBV	244	305	0.03%	0.004%
22	4.608	1020	1032	1064	rBV	62057	182862	17.85%	2.304%
23	4.881	1115	1117	1120	rVB2	304	149	0.01%	0.002%
24	5.052	1154	1170	1193	rBV	177638	398104	38.85%	5.015%
25	5.158	1200	1203	1209	rVB4	616	439	0.04%	0.006%
26	5.248	1229	1231	1234	rBV	292	209	0.02%	0.003%
27	5.550	1322	1325	1329	rVB2	212	138	0.01%	0.002%
28	5.627	1346	1349	1352	rVB	237	164	0.02%	0.002%
29	5.650	1352	1356	1357	rBV	231	191	0.02%	0.002%
30	5.714	1357	1376	1399	rBV2	376530	1024630	100.00%	12.908%
31	6.242	1526	1540	1569	rBV	370114	722541	70.52%	9.102%
32	6.524	1621	1628	1638	rVB6	1322	1984	0.19%	0.025%
33	6.682	1661	1677	1699	rBV	232490	460411	44.93%	5.800%
34	6.942	1753	1758	1763	rVB2	290	390	0.04%	0.005%
35	6.978	1763	1769	1772	rBV2	243	258	0.03%	0.003%
36	7.000	1772	1776	1777	rBV	211	163	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057905.D
 Acq On : 20 Feb 2024 16:18
 Operator : MD/SY
 Sample : P1513-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

37	7.042	1785	1789	1791	rBV2	204	190	0.02%	0.002%
38	7.196	1833	1837	1839	rBV2	431	294	0.03%	0.004%
39	7.335	1877	1880	1884	rVB	194	134	0.01%	0.002%
40	7.505	1931	1933	1936	rVB2	319	191	0.02%	0.002%
41	7.560	1936	1950	1972	rBV	128300	235713	23.00%	2.969%
42	7.704	1991	1995	1998	rBV4	338	259	0.03%	0.003%
43	7.753	2007	2010	2014	rVB2	283	228	0.02%	0.003%
44	7.791	2019	2022	2026	rBV2	166	152	0.01%	0.002%
45	7.891	2039	2053	2090	rBV	468238	824624	80.48%	10.388%
46	8.106	2117	2120	2126	rVB2	525	526	0.05%	0.007%
47	8.174	2130	2141	2168	rBV	86886	156521	15.28%	1.972%
48	8.463	2226	2231	2236	rBV2	313	356	0.03%	0.004%
49	8.560	2259	2261	2267	rVB2	220	198	0.02%	0.002%
50	8.627	2270	2282	2318	rBV2	201310	428459	41.82%	5.398%
51	8.933	2374	2377	2382	rVV2	124	139	0.01%	0.002%
52	9.126	2434	2437	2438	rBV	267	137	0.01%	0.002%
53	9.338	2500	2503	2508	rVB2	196	165	0.02%	0.002%
54	9.367	2508	2512	2513	rBV	190	136	0.01%	0.002%
55	9.412	2513	2526	2554	rBV	517550	883044	86.18%	11.124%
56	9.621	2588	2591	2593	rBV	250	137	0.01%	0.002%
57	9.814	2647	2651	2653	rBV	203	181	0.02%	0.002%
58	10.335	2809	2813	2815	rBV	153	155	0.02%	0.002%
59	10.563	2878	2884	2886	rBV	239	273	0.03%	0.003%
60	10.627	2901	2904	2907	rBV	293	222	0.02%	0.003%
61	10.675	2916	2919	2923	rVB	207	188	0.02%	0.002%
62	10.698	2923	2926	2929	rBV2	246	208	0.02%	0.003%
63	10.749	2929	2942	2963	rVV	270696	444145	43.35%	5.595%
64	10.897	2981	2988	2990	rBV3	329	360	0.04%	0.005%
65	10.962	3003	3008	3011	rBV2	224	213	0.02%	0.003%
66	10.984	3011	3015	3019	rVV2	197	196	0.02%	0.002%
67	11.055	3034	3037	3039	rBV	245	149	0.01%	0.002%
68	11.087	3042	3047	3049	rBV	212	216	0.02%	0.003%
69	11.222	3086	3089	3093	rVB	193	186	0.02%	0.002%
70	11.306	3112	3115	3118	rVB	241	141	0.01%	0.002%
71	11.434	3151	3155	3158	rBV2	246	220	0.02%	0.003%
72	11.608	3206	3209	3212	rBV	167	137	0.01%	0.002%
73	11.646	3217	3221	3222	rBV	201	141	0.01%	0.002%
74	11.807	3258	3271	3300	rVV	512771	834484	81.44%	10.513%
75	12.187	3376	3389	3413	rBV	401921	677574	66.13%	8.536%
76	12.328	3430	3433	3436	rVB2	333	170	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
 Data File : VU057905.D
 Acq On : 20 Feb 2024 16:18
 Operator : MD/SY
 Sample : P1513-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

77	12.405	3454	3457	3460	rBV3	415	343	0.03%	0.004%
78	12.466	3471	3476	3481	rBV2	259	378	0.04%	0.005%
79	12.730	3555	3558	3560	rBV	242	159	0.02%	0.002%
80	12.807	3578	3582	3585	rBV2	205	181	0.02%	0.002%
81	12.913	3612	3615	3618	rBV	223	163	0.02%	0.002%
82	12.965	3628	3631	3634	rBV2	152	141	0.01%	0.002%
83	13.032	3650	3652	3660	rVB2	537	585	0.06%	0.007%
84	13.071	3660	3664	3666	rBV2	275	277	0.03%	0.003%
85	13.592	3824	3826	3829	rVB	344	184	0.02%	0.002%
86	13.736	3865	3871	3872	rBV	217	229	0.02%	0.003%
87	13.833	3898	3901	3903	rBV2	240	167	0.02%	0.002%
88	13.997	3949	3952	3955	rVB2	327	232	0.02%	0.003%
89	14.129	3989	3993	3997	rBV3	336	348	0.03%	0.004%
90	14.199	4009	4015	4017	rBV3	253	251	0.02%	0.003%
91	14.251	4022	4031	4034	rBV2	323	481	0.05%	0.006%
92	14.399	4073	4077	4079	rBV2	318	270	0.03%	0.003%
93	14.527	4114	4117	4119	rBV	238	185	0.02%	0.002%
94	14.662	4153	4159	4162	rBV3	318	390	0.04%	0.005%
95	14.762	4187	4190	4195	rBV2	286	324	0.03%	0.004%
96	14.855	4216	4219	4221	rBV2	265	211	0.02%	0.003%
97	15.212	4325	4330	4335	rVB3	368	349	0.03%	0.004%
98	15.244	4335	4340	4344	rBV3	455	550	0.05%	0.007%
99	15.395	4384	4387	4390	rBV	339	187	0.02%	0.002%
100	16.174	4626	4629	4633	rBV3	609	596	0.06%	0.008%




Sum of corrected areas: 7937907

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057905.D
Acq On : 20 Feb 2024 16:18
Operator : MD/SY
Sample : P1513-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

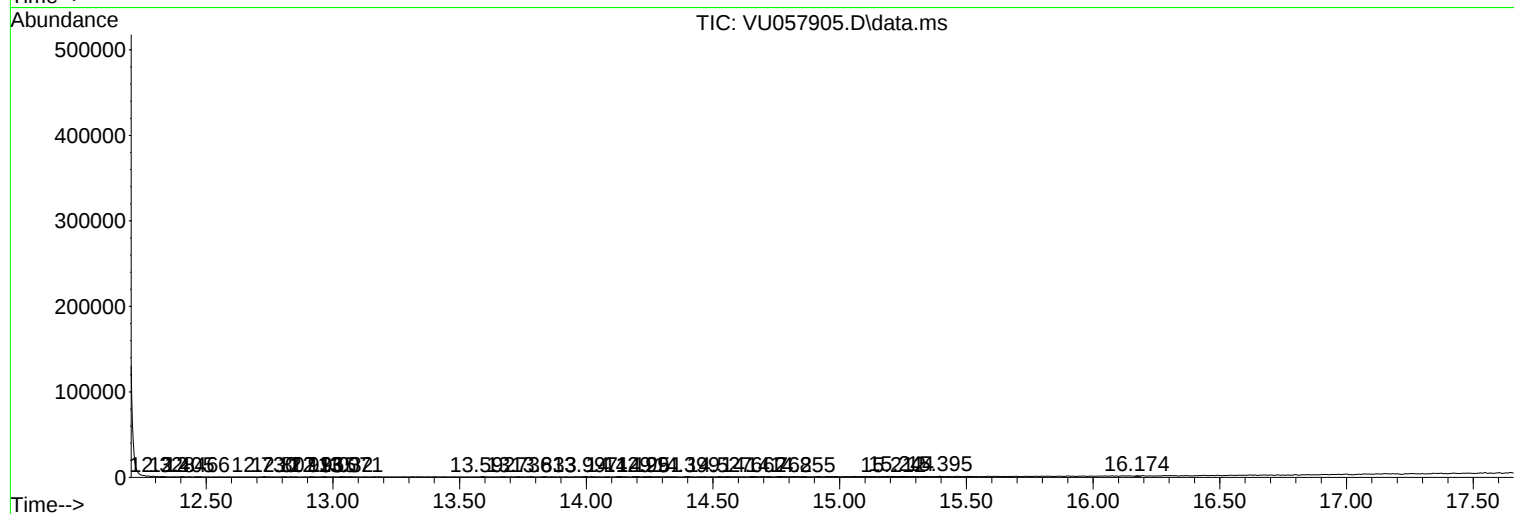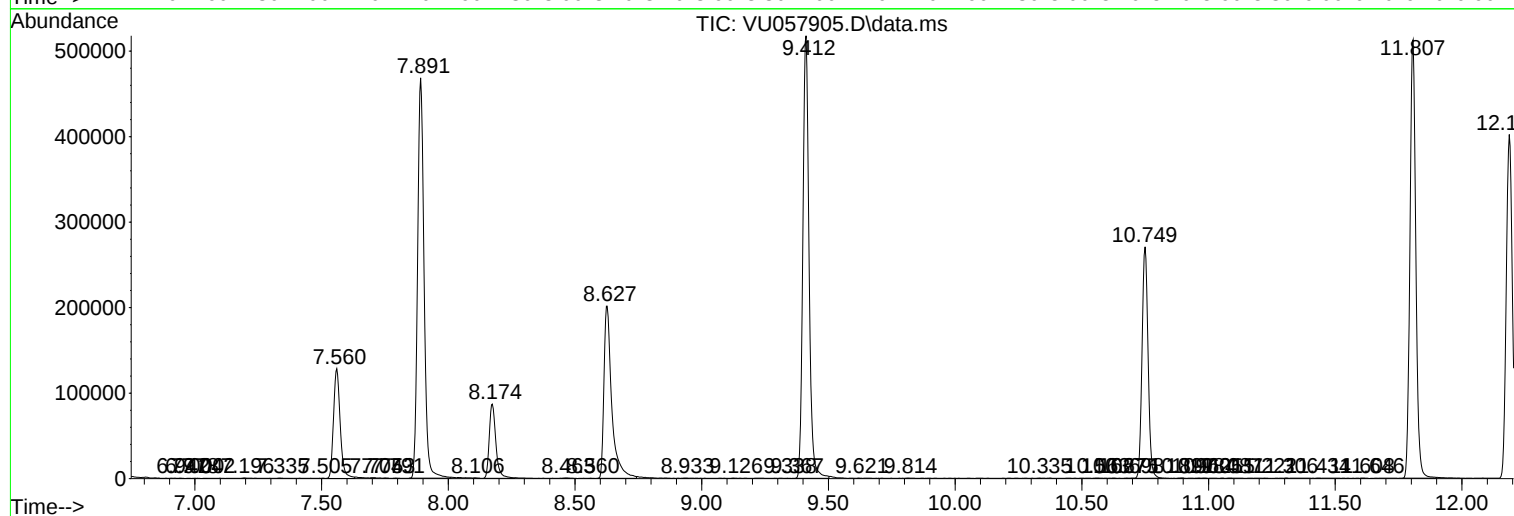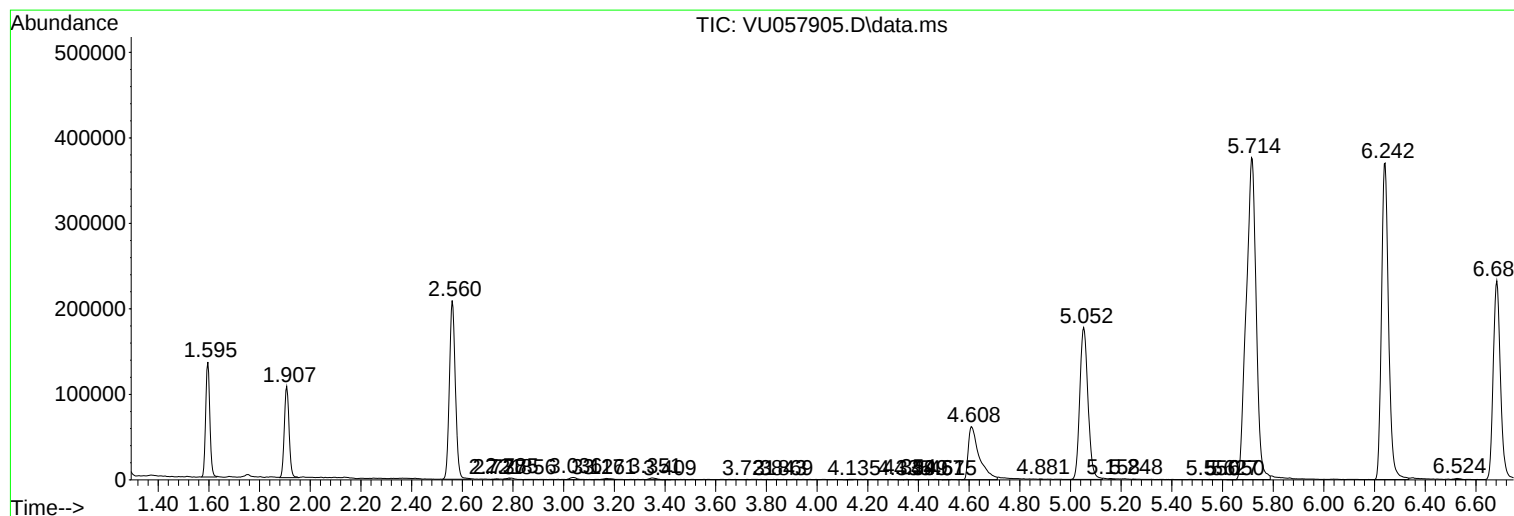

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057905.D
Acq On : 20 Feb 2024 16:18
Operator : MD/SY
Sample : P1513-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057905.D
Acq On : 20 Feb 2024 16:18
Operator : MD/SY
Sample : P1513-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------