


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022024\
Data File : VU057888.D
Acq On : 20 Feb 2024 08:32
Operator : MD/SY
Sample : BFB040
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB040

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Title : VOC Analysis
Last Update : Wed Feb 21 00:11:26 2024

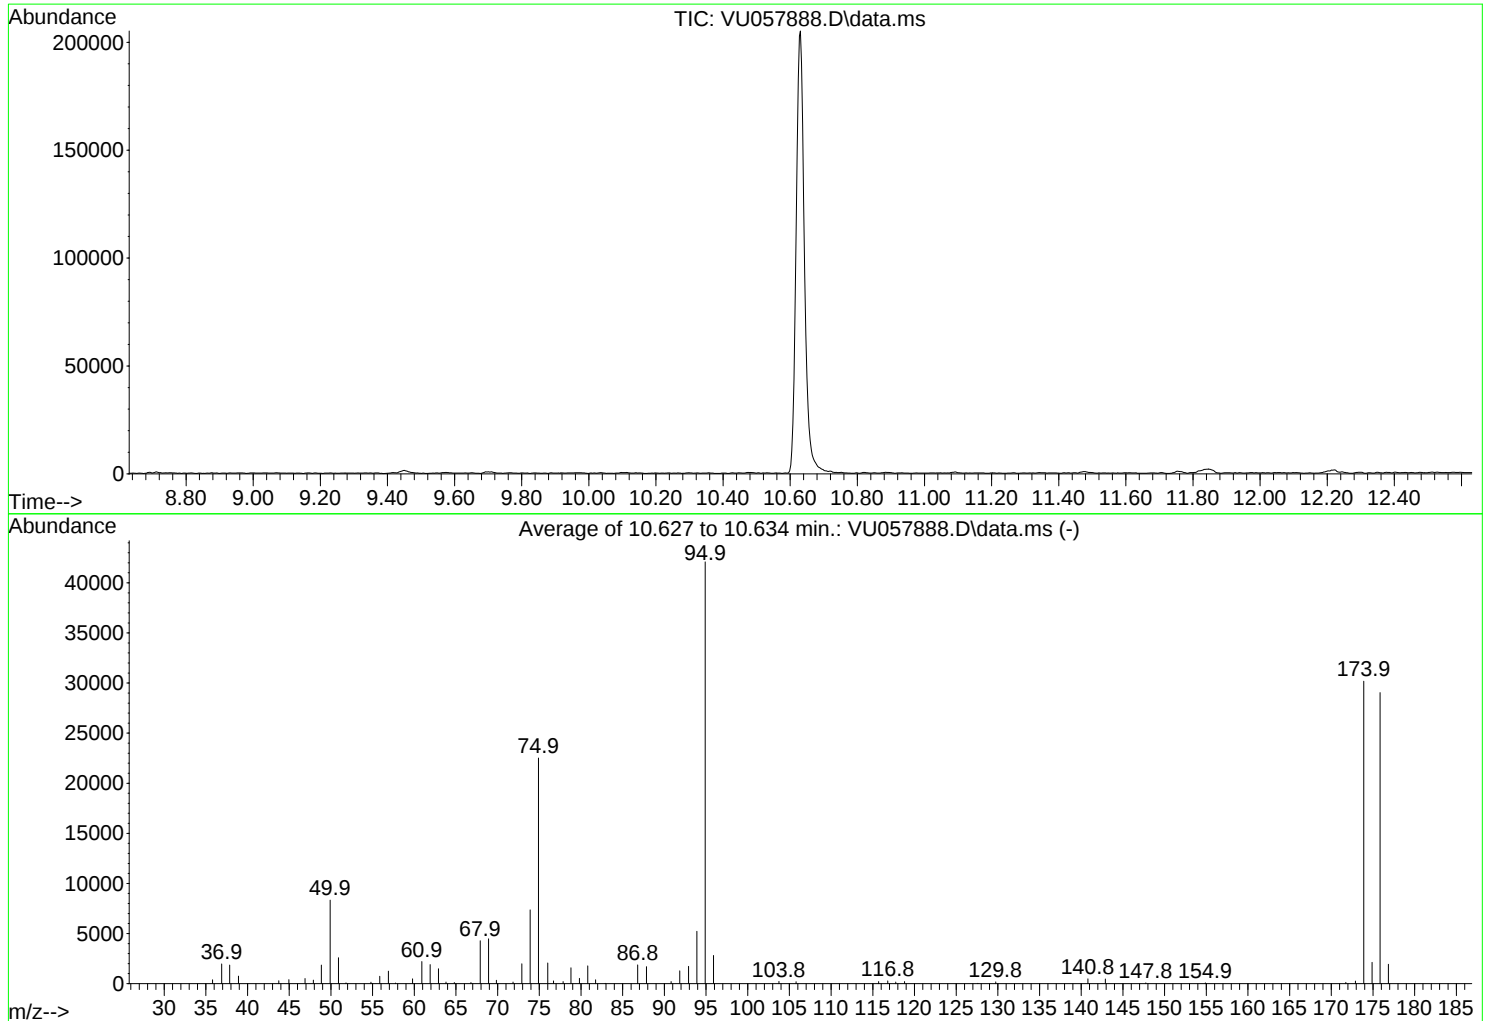

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	8329	PASS
75	95	30	80	53.5	22515	PASS
95	95	100	100	100.0	42096	PASS
96	95	5	9	6.7	2815	PASS
173	174	0.00	2	0.8	256	PASS
174	95	50	120	71.7	30179	PASS
175	174	5	9	7.0	2122	PASS
176	174	95	101	96.3	29048	PASS
177	176	5	9	6.7	1932	PASS

m/z	Abundance
39.90	103.0
43.80	249.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
35.80	395.0
36.90	1998.0
37.90	1925.0
38.90	839.0
43.80	546.0
45.00	427.0
46.90	460.0
47.90	390.0
48.90	1852.0
49.90	8800.0
50.90	2535.0
51.80	144.0
54.80	145.0
55.80	743.0
56.90	1277.0
57.70	106.0
59.80	477.0
60.90	2172.0
61.90	1972.0
62.90	1539.0
63.80	174.0
64.80	100.0
66.90	115.0
67.90	4426.0
68.90	4549.0
69.90	350.0
71.80	205.0
72.90	2034.0
73.90	7641.0
74.90	23360.0
76.00	2076.0
76.70	294.0
77.80	246.0
78.80	1584.0
79.80	536.0
80.80	1760.0
81.80	416.0
86.80	1991.0
87.90	1679.0
90.80	211.0
91.80	1277.0
92.90	1618.0
93.90	5288.0
94.90	42536.0
95.90	2901.0
103.70	259.0
105.80	200.0
115.70	227.0
116.80	267.0
117.70	163.0
118.80	204.0
129.80	208.0
140.80	552.0
142.90	455.0
147.80	128.0
154.90	129.0
171.70	133.0
172.90	254.0
173.90	30456.0
174.90	2199.0
175.90	29120.0
176.90	1852.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
35.90	398.0
36.90	1990.0
37.90	1895.0
38.90	764.0
39.90	100.0
43.70	551.0
44.90	419.0
46.90	507.0
47.90	382.0
48.80	1897.0
49.90	8479.0
50.90	2632.0
51.80	122.0
54.80	133.0
55.90	773.0
56.90	1285.0
57.80	106.0
59.80	521.0
60.90	2272.0
61.90	1907.0
62.90	1509.0
63.80	179.0
64.80	126.0
66.80	110.0
67.90	4419.0
68.90	4590.0
69.90	358.0
71.80	159.0
72.90	2050.0
73.90	7592.0
74.90	23064.0
76.00	2143.0
76.70	294.0
77.90	219.0
78.80	1650.0
79.80	539.0
80.80	1781.0
81.80	398.0
86.80	1921.0
87.90	1719.0
90.80	213.0
91.90	1308.0
92.90	1758.0
93.90	5384.0
94.90	43352.0
95.90	2901.0
103.80	222.0
105.80	213.0
115.70	232.0
116.80	288.0
117.80	172.0
118.80	214.0
129.70	185.0
140.80	490.0
142.90	480.0
147.70	107.0
154.90	101.0
171.70	126.0
172.90	270.0
173.90	31160.0
174.90	2171.0
175.90	29840.0
176.90	2057.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
35.80	355.0
36.90	1889.0
37.80	1748.0
38.90	637.0
39.90	139.0
43.80	525.0
44.90	367.0
46.90	560.0
47.90	306.0
48.80	1789.0
49.90	7707.0
50.90	2572.0
54.80	136.0
55.90	669.0
56.90	1189.0
59.80	460.0
60.90	2185.0
61.90	1805.0
62.90	1410.0
63.80	144.0
64.80	137.0
66.70	110.0
67.90	3996.0
68.90	4270.0
69.80	322.0
71.90	123.0
72.90	1877.0
73.90	6850.0
74.90	21120.0
76.00	1956.0
76.70	236.0
77.90	173.0
78.80	1528.0
79.80	488.0
80.80	1765.0
81.70	337.0
82.90	101.0
86.80	1686.0
87.80	1670.0
90.80	208.0
91.90	1258.0
92.90	1779.0
93.90	5015.0
94.90	40400.0
95.90	2642.0
103.80	181.0
105.80	184.0
115.70	172.0
116.80	279.0
117.80	162.0
118.80	211.0
127.60	113.0
129.70	158.0
140.80	416.0
142.90	447.0
171.80	111.0
172.90	243.0
173.90	28920.0
174.90	1995.0
175.80	28184.0
176.80	1887.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040