

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU022119\
 Data File : VU029598.D
 Acq On : 21 Feb 2019 15:23
 Operator : JC/SP
 Sample : K1488-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESXC7

Quant Time: Feb 22 03:41:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Feb 22 03:07:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	229404	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	225959	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	113718	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	72972	4.87	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.40%
7) Chloroethane-d5	1.68	69	69528	4.93	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.60%
11) 1,1-Dichloroethene-d2	2.27	63	117271	3.64	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.80%
20) 2-Butanone-d5	4.19	46	180464	53.28	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.56%
24) Chloroform-d	4.65	84	135777	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.80%
26) 1,2-Dichloroethane-d4	5.31	65	72359	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.60%
32) Benzene-d6	5.34	84	289944	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.00%
36) 1,2-Dichloropropane-d6	6.33	67	88069	5.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.40%
41) Toluene-d8	7.56	98	276317	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.20%
43) trans-1,3-Dichloropropene-	7.85	79	32968	4.76	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.20%
46) 2-Hexanone-d5	8.31	63	178303	52.50	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.00%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	73829	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.40%
64) 1,2-Dichlorobenzene-d4	11.86	152	118961	5.32	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.40%


Target Compounds					Ovalue
13) Acetone	2.32	43	6097	2.505 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU022119\
Data File : VU029598.D
Acq On : 21 Feb 2019 15:23
Operator : JC/SP
Sample : K1488-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESXC7

Quant Time: Feb 22 03:41:03 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Feb 22 03:07:37 2019
Response via : Initial Calibration

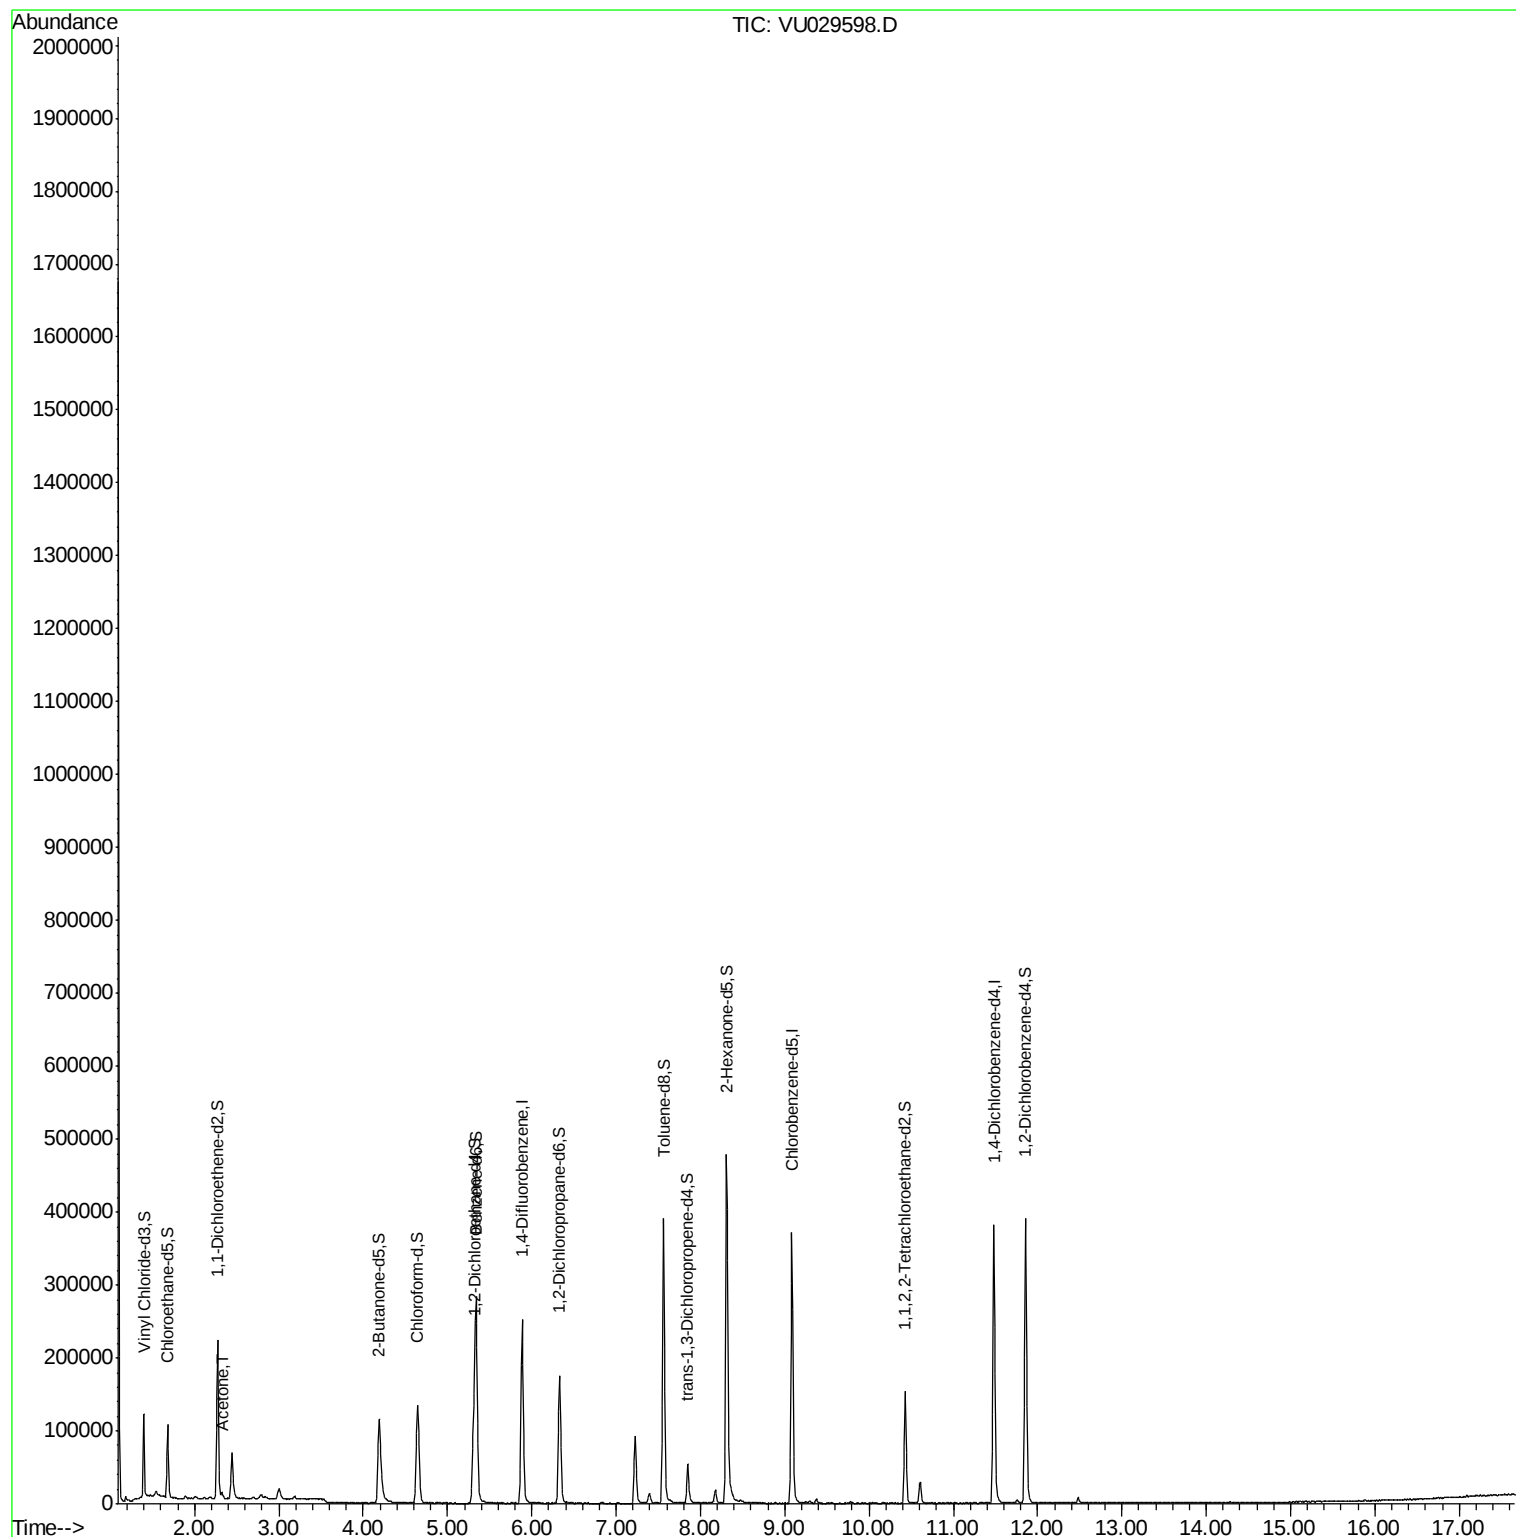

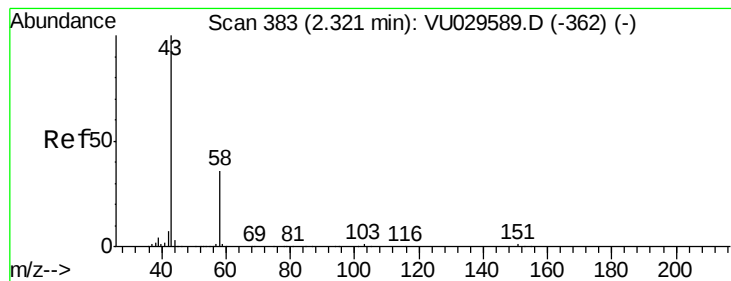

#13

Acetone

Concen: 2.505 ug/L

RT: 2.32 min Scan# 384

Delta R.T. 0.00 min

Lab File: VU029598.D

Acq: 21 Feb 2019 15:23

Instrument :
MSVOA_U
ClientSampleId :
ESXC7

Tot Ion: 43 Resp: 6097

Ion Ratio Lower Upper

43 100

58 39.4 0.0 70.2

