


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU022119\
 Data File : VU029586.D
 Acq On : 21 Feb 2019 10:09
 Operator : JC/SP
 Sample : BFB47
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB47

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Feb 22 03:07:37 2019

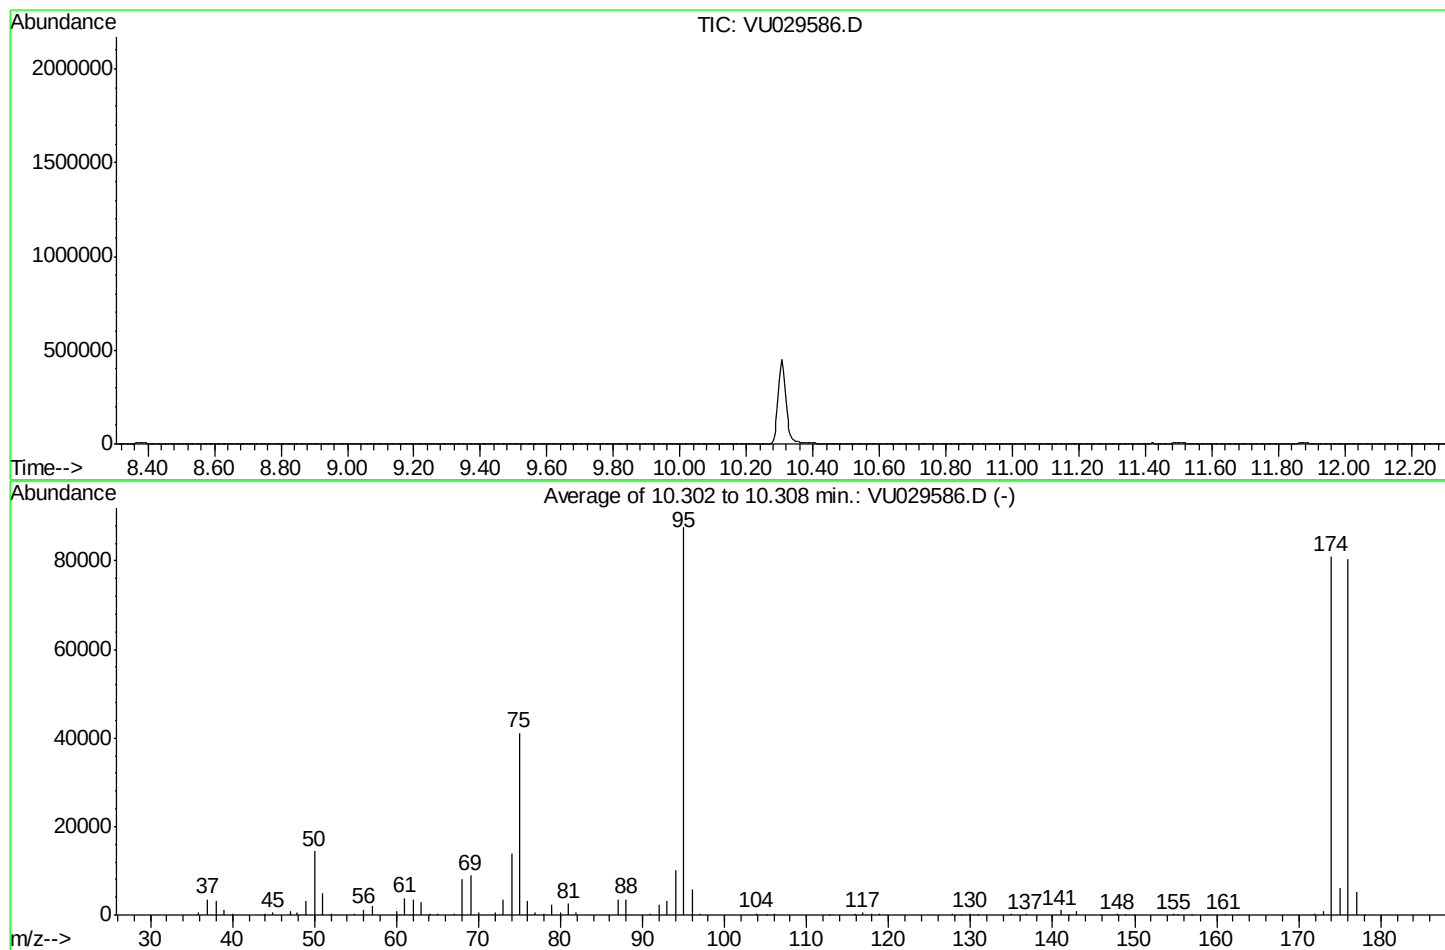

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	14395	PASS
75	95	30	80	46.9	41064	PASS
95	95	100	100	100.0	87581	PASS
96	95	5	9	6.6	5794	PASS
173	174	0.00	2	0.9	743	PASS
174	95	50	120	92.4	80893	PASS
175	174	5	9	7.5	6061	PASS
176	174	95	101	99.2	80277	PASS
177	176	5	9	6.3	5090	PASS

Scan 2852 (10.260 min): VU029586.D
BFB47

m/z	Abundance
44.00	536.0
206.90	182.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
35.90	600.0
37.00	3338.0
38.00	3085.0
39.00	1207.0
40.00	224.0
43.90	961.0
45.00	598.0
47.00	812.0
47.90	447.0
49.00	3093.0
50.00	13937.0
51.00	4607.0
52.00	210.0
54.90	221.0
56.00	1140.0
57.00	2168.0
60.00	803.0
61.00	3815.0
62.00	3672.0
63.10	2718.0
64.10	308.0
65.10	187.0
67.00	212.0
68.00	8097.0
69.00	8517.0
70.10	513.0
72.00	463.0
73.00	3355.0
74.00	13603.0
75.00	40384.0
76.00	3030.0
77.00	541.0
78.00	329.0
78.90	2171.0
79.90	675.0
81.00	2534.0
81.90	529.0
87.00	3214.0
88.00	3469.0
90.90	309.0
92.00	2193.0
93.00	3052.0
94.00	9648.0
95.00	83472.0
96.00	5596.0
97.00	203.0
103.90	325.0
106.00	290.0
112.80	119.0
115.90	345.0
116.90	537.0
117.90	272.0
118.90	399.0
127.80	289.0
128.90	129.0
129.90	349.0
130.90	133.0
135.00	121.0
136.80	179.0
140.90	976.0
142.90	784.0
147.90	237.0
148.80	100.0
149.90	106.0
154.80	239.0
157.00	157.0
161.00	134.0
171.90	260.0
172.90	633.0
174.00	75352.0
175.00	5711.0
176.00	75224.0
177.00	4762.0
178.00	128.0
206.90	167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
35.00	629.0
37.00	3616.0
38.00	3368.0
39.00	1341.0
40.00	243.0
43.90	976.0
45.00	529.0
47.00	933.0
47.90	479.0
49.00	3233.0
50.00	14838.0
51.00	5009.0
52.00	282.0
54.90	231.0
56.00	1252.0
57.00	2236.0
59.90	774.0
61.00	4020.0
62.00	3651.0
63.00	3123.0
64.00	306.0
65.10	154.0
67.10	276.0
68.00	8453.0
69.00	9211.0
70.10	600.0
72.00	499.0
73.00	3636.0
74.00	14463.0
75.00	42408.0
76.00	3318.0
76.90	569.0
78.00	450.0
78.90	2297.0
79.90	719.0
81.00	2689.0
81.90	578.0
87.00	3510.0
88.00	3609.0
91.00	405.0
92.00	2344.0
93.00	3245.0
94.00	10314.0
95.00	90624.0
96.00	6017.0
97.00	219.0
103.90	325.0
105.00	118.0
106.00	328.0
116.00	405.0
116.90	525.0
117.90	286.0
118.90	401.0
127.80	310.0
128.90	136.0
130.00	412.0
131.00	161.0
134.90	160.0
136.80	177.0
141.00	1139.0
141.90	101.0
142.90	916.0
147.90	256.0
148.80	106.0
149.80	114.0
154.80	202.0
156.90	129.0
161.00	150.0
171.90	361.0
172.90	740.0
174.00	83304.0
175.00	6246.0
176.00	82848.0
177.00	5283.0
178.00	157.0
207.00	164.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
35.90	626.0
37.00	3520.0
38.00	3264.0
39.00	1333.0
40.00	207.0
44.00	976.0
44.90	491.0
47.00	902.0
47.90	465.0
49.00	3146.0
50.00	14412.0
51.00	4918.0
52.00	308.0
54.80	212.0
56.00	1209.0
57.10	2110.0
59.90	718.0
61.00	3724.0
62.00	3312.0
63.00	3249.0
64.00	291.0
65.00	134.0
67.10	278.0
68.00	8104.0
69.00	9060.0
70.00	634.0
72.00	482.0
73.00	3536.0
74.00	13977.0
75.00	40400.0
76.00	3305.0
76.90	517.0
78.00	412.0
78.90	2315.0
80.00	731.0
81.00	2460.0
81.90	568.0
87.00	3498.0
88.00	3442.0
91.00	431.0
92.00	2359.0
93.00	3296.0
94.00	10195.0
95.00	88648.0
96.00	5771.0
97.00	183.0
103.90	364.0
105.10	151.0
106.00	315.0
116.00	423.0
116.90	514.0
117.90	275.0
118.90	424.0
127.80	333.0
128.90	121.0
130.00	402.0
131.00	149.0
134.90	223.0
136.80	174.0
140.90	1062.0
141.90	102.0
142.90	952.0
145.90	130.0
147.90	253.0
154.80	174.0
155.20	122.0
160.90	129.0
171.90	403.0
173.00	857.0
174.00	84024.0
175.00	6227.0
176.00	82760.0
177.00	5225.0
178.00	154.0
207.00	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47