


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU022120\
 Data File : VU036872.D
 Acq On : 21 Feb 2020 09:13
 Operator : JC/MD
 Sample : BFB12
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB12

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Feb 22 00:05:53 2020

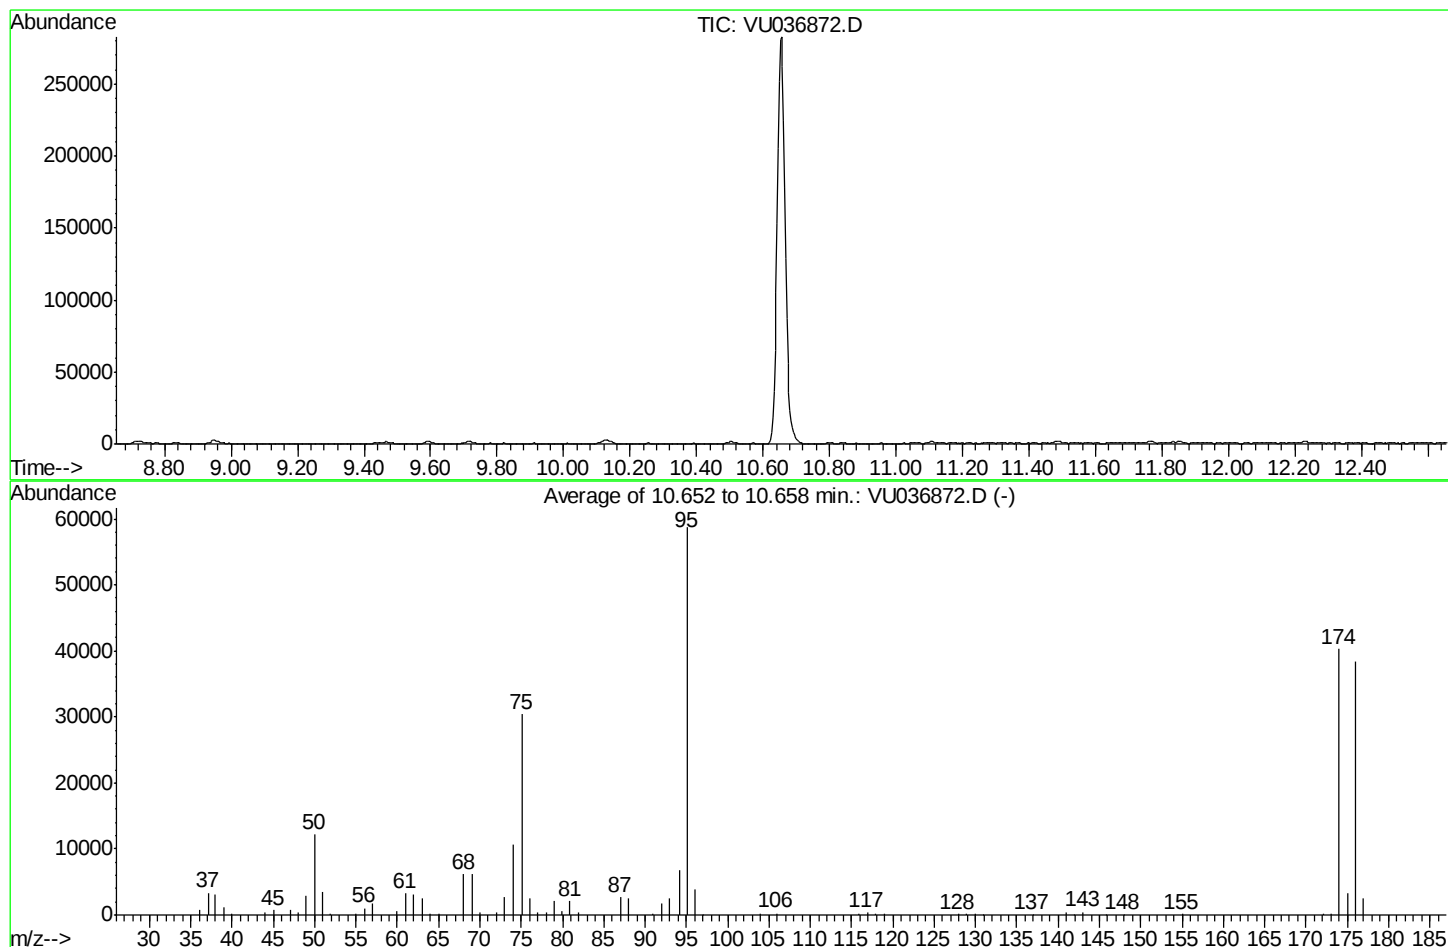

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	12187	PASS
75	95	30	80	51.7	30381	PASS
95	95	100	100	100.0	58709	PASS
96	95	5	9	6.5	3800	PASS
173	174	0.00	2	0.5	212	PASS
174	95	50	120	68.6	40272	PASS
175	174	5	9	8.1	3269	PASS
176	174	95	101	95.3	38386	PASS
177	176	5	9	6.5	2493	PASS

m/z	Abundance
36.00	738.0
37.10	3433.0
38.00	3028.0
39.00	1034.0
39.90	110.0
44.00	849.0
45.00	752.0
47.00	788.0
48.00	451.0
49.00	2983.0
50.00	12503.0
51.00	3680.0
51.90	203.0
54.90	198.0
56.00	1020.0
57.00	1786.0
60.00	620.0
61.00	3381.0
62.00	3264.0
63.00	2458.0
64.00	242.0
65.10	138.0
68.00	6380.0
69.00	6271.0
70.00	396.0
72.00	406.0
73.00	2754.0
74.10	10824.0
75.00	31496.0
76.10	2582.0
77.00	353.0
78.20	343.0
78.90	2240.0
79.90	651.0
80.90	2271.0
81.90	484.0
87.00	2765.0
88.00	2527.0
90.90	193.0
92.00	1683.0
93.00	2580.0
94.10	7058.0
95.10	60112.0
96.10	3852.0
97.00	105.0
103.90	292.0
105.90	272.0
115.90	247.0
117.00	305.0
117.90	216.0
118.90	225.0
127.90	195.0
128.90	119.0
129.90	136.0
130.90	103.0
136.90	144.0
140.90	486.0
141.90	113.0
143.00	429.0
145.80	105.0
147.90	110.0
155.00	128.0
172.00	179.0
173.10	636.0
174.00	40120.0
175.00	3349.0
176.00	38312.0
177.00	2455.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
36.00	759.0
37.10	3472.0
38.00	3121.0
38.90	1213.0
39.90	106.0
44.00	848.0
45.00	729.0
47.00	872.0
48.00	482.0
49.00	3082.0
50.00	12484.0
51.00	3466.0
51.90	198.0
55.00	158.0
56.00	1053.0
57.00	1770.0
60.00	670.0
61.00	3389.0
62.00	3220.0
63.00	2516.0
64.00	217.0
65.00	165.0
68.00	6409.0
69.00	6288.0
70.00	467.0
72.00	377.0
73.00	2848.0
74.10	11057.0
75.10	31136.0
76.00	2628.0
77.00	338.0
78.10	314.0
79.00	2238.0
79.90	613.0
80.90	2152.0
81.90	495.0
87.00	2726.0
88.00	2492.0
91.00	208.0
92.00	1797.0
93.00	2588.0
94.10	7010.0
95.10	60312.0
96.10	3926.0
103.90	278.0
105.90	279.0
115.90	239.0
117.00	337.0
117.90	229.0
118.90	223.0
127.90	196.0
128.90	129.0
129.90	174.0
130.90	102.0
136.90	112.0
141.00	465.0
143.00	477.0
155.00	132.0
172.10	188.0
174.00	41408.0
175.00	3376.0
176.00	39504.0
177.00	2536.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
36.00	707.0
37.10	3134.0
38.00	2887.0
38.90	1110.0
39.90	109.0
44.00	757.0
45.10	643.0
47.00	861.0
48.10	433.0
49.00	2873.0
50.00	11574.0
51.00	3210.0
52.00	147.0
55.00	140.0
56.00	969.0
57.00	1641.0
60.00	616.0
61.00	3020.0
62.00	2963.0
63.00	2329.0
64.00	180.0
65.00	169.0
68.00	5776.0
69.00	5817.0
70.00	514.0
72.00	342.0
73.00	2656.0
74.10	10142.0
75.10	28512.0
76.00	2372.0
76.90	320.0
78.00	276.0
79.00	1994.0
80.00	538.0
80.90	1876.0
81.90	439.0
87.00	2529.0
88.00	2364.0
91.00	234.0
92.00	1726.0
93.00	2297.0
94.10	6541.0
95.10	55704.0
96.10	3622.0
97.00	115.0
103.90	240.0
105.90	295.0
115.90	208.0
116.90	377.0
117.90	194.0
118.90	223.0
127.90	171.0
128.90	103.0
129.90	209.0
141.00	429.0
143.00	489.0
155.00	102.0
172.10	232.0
174.00	39288.0
175.00	3082.0
176.00	37344.0
177.00	2490.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
43.90	347.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12