

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022124\
 Data File : VU057914.D
 Acq On : 21 Feb 2024 10:30
 Operator : MD/SY
 Sample : VU0221WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK042

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

Signal : TIC: VU057914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	112	rVB	126581	142192	14.85%	1.920%
2	1.907	184	192	203	rBV	99404	123141	12.86%	1.663%
3	2.560	383	395	417	rBV	194765	324061	33.84%	4.376%
4	2.788	458	466	477	rVB3	2118	3781	0.39%	0.051%
5	2.949	514	516	523	rVB2	299	278	0.03%	0.004%
6	3.039	535	544	553	rVB3	2141	3522	0.37%	0.048%
7	3.165	579	583	584	rBV3	395	258	0.03%	0.003%
8	3.296	619	624	629	rBV	236	251	0.03%	0.003%
9	3.348	629	640	641	rBV2	1145	1158	0.12%	0.016%
10	3.502	685	688	691	rBV2	248	218	0.02%	0.003%
11	3.570	704	709	711	rBV	243	236	0.02%	0.003%
12	3.949	824	827	831	rBV2	193	190	0.02%	0.003%
13	3.972	831	834	839	rVV2	193	222	0.02%	0.003%
14	4.087	867	870	876	rVB2	243	285	0.03%	0.004%
15	4.116	876	879	883	rVB	284	194	0.02%	0.003%
16	4.148	883	889	891	rBV	277	291	0.03%	0.004%
17	4.248	917	920	927	rVB	222	211	0.02%	0.003%
18	4.329	942	945	948	rBV2	208	191	0.02%	0.003%
19	4.409	963	970	979	rBV2	362	548	0.06%	0.007%
20	4.473	986	990	998	rBV2	340	427	0.04%	0.006%
21	4.525	1004	1006	1012	rVB	195	186	0.02%	0.003%
22	4.608	1023	1032	1065	rBV	53517	147095	15.36%	1.986%
23	4.975	1142	1146	1149	rBV3	370	354	0.04%	0.005%
24	5.052	1155	1170	1193	rBV	167871	374707	39.13%	5.060%
25	5.203	1215	1217	1227	rVB5	726	981	0.10%	0.013%
26	5.325	1252	1255	1258	rVB2	326	242	0.03%	0.003%
27	5.534	1315	1320	1322	rBV2	215	217	0.02%	0.003%
28	5.624	1344	1348	1353	rBV	201	203	0.02%	0.003%
29	5.718	1356	1377	1407	rBV2	346138	957561	100.00%	12.930%
30	5.981	1456	1459	1462	rBV2	305	254	0.03%	0.003%
31	6.242	1525	1540	1573	rBV	348987	688097	71.86%	9.291%
32	6.537	1622	1632	1642	rVB7	1843	3488	0.36%	0.047%
33	6.682	1663	1677	1698	rBV	217073	433212	45.24%	5.850%
34	6.943	1755	1758	1763	rBV	281	178	0.02%	0.002%
35	7.000	1773	1776	1781	rBV2	218	209	0.02%	0.003%
36	7.065	1790	1796	1798	rBV2	172	190	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022124\
 Data File : VU057914.D
 Acq On : 21 Feb 2024 10:30
 Operator : MD/SY
 Sample : VU0221WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK042

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

37	7.200	1832	1838	1840	rBV2	398	422	0.04%	0.006%
38	7.306	1868	1871	1875	rBV2	258	262	0.03%	0.004%
39	7.348	1880	1884	1890	rBV2	211	271	0.03%	0.004%
40	7.557	1938	1949	1979	rBV	115823	218974	22.87%	2.957%
41	7.676	1979	1986	1994	rVB5	2275	3853	0.40%	0.052%
42	7.791	2015	2022	2025	rBV5	650	819	0.09%	0.011%
43	7.891	2039	2053	2093	rBV	424325	764028	79.79%	10.316%
44	8.129	2124	2127	2130	rBV2	204	184	0.02%	0.002%
45	8.174	2130	2141	2163	rBV	77838	141555	14.78%	1.911%
46	8.467	2225	2232	2235	rBV2	471	632	0.07%	0.009%
47	8.550	2252	2258	2261	rVV4	823	729	0.08%	0.010%
48	8.627	2271	2282	2323	rBV2	160748	365904	38.21%	4.941%
49	8.897	2363	2366	2369	rVB	305	184	0.02%	0.002%
50	8.920	2369	2373	2374	rBV2	508	354	0.04%	0.005%
51	9.013	2398	2402	2405	rBV2	364	336	0.04%	0.005%
52	9.032	2405	2408	2412	rVV	297	261	0.03%	0.004%
53	9.315	2492	2496	2500	rBV	268	269	0.03%	0.004%
54	9.409	2513	2525	2567	rBV	473809	842185	87.95%	11.372%
55	9.566	2572	2574	2583	rVV3	1111	1465	0.15%	0.020%
56	9.688	2607	2612	2614	rBV3	818	731	0.08%	0.010%
57	10.049	2720	2724	2727	rBV	234	222	0.02%	0.003%
58	10.068	2727	2730	2733	rVB	295	211	0.02%	0.003%
59	10.097	2733	2739	2743	rBV3	652	873	0.09%	0.012%
60	10.126	2743	2748	2752	rVB3	752	949	0.10%	0.013%
61	10.405	2828	2835	2839	rBV2	323	426	0.04%	0.006%
62	10.483	2854	2859	2868	rVB2	882	1280	0.13%	0.017%
63	10.569	2881	2886	2892	rVB2	226	278	0.03%	0.004%
64	10.598	2892	2895	2901	rVB2	191	236	0.02%	0.003%
65	10.634	2901	2906	2910	rBV2	360	453	0.05%	0.006%
66	10.749	2929	2942	2959	rBV	242246	400400	41.81%	5.406%
67	10.849	2971	2973	2977	rVB2	273	209	0.02%	0.003%
68	11.090	3039	3048	3053	rBV3	966	1712	0.18%	0.023%
69	11.148	3063	3066	3073	rBV2	300	405	0.04%	0.005%
70	11.393	3136	3142	3145	rBV2	260	195	0.02%	0.003%
71	11.473	3158	3167	3177	rBB3	1239	1884	0.20%	0.025%
72	11.647	3215	3221	3224	rVB2	207	220	0.02%	0.003%
73	11.746	3244	3252	3259	rBV2	2593	3347	0.35%	0.045%
74	11.804	3259	3270	3294	rBV	465722	772368	80.66%	10.429%
75	11.994	3324	3329	3332	rBV2	273	329	0.03%	0.004%
76	12.010	3332	3334	3340	rVV2	309	257	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022124\
 Data File : VU057914.D
 Acq On : 21 Feb 2024 10:30
 Operator : MD/SY
 Sample : VU0221WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK042

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

77	12.048	3343	3346	3348	rBV	291	206	0.02%	0.003%
78	12.065	3348	3351	3360	rBV2	173	218	0.02%	0.003%
79	12.187	3376	3389	3410	rBV	370145	616678	64.40%	8.327%
80	12.634	3521	3528	3532	rBV2	288	396	0.04%	0.005%
81	13.183	3695	3699	3701	rBV2	365	334	0.03%	0.005%
82	13.228	3704	3713	3724	rVB5	2745	4813	0.50%	0.065%
83	13.418	3768	3772	3778	rBV2	157	197	0.02%	0.003%
84	13.470	3785	3788	3793	rBV	322	323	0.03%	0.004%
85	13.708	3859	3862	3865	rBV	281	217	0.02%	0.003%
86	13.846	3895	3905	3918	rBV3	6644	11321	1.18%	0.153%
87	14.093	3972	3982	3995	rBV	8003	16450	1.72%	0.222%
88	14.328	4046	4055	4068	rVV4	7225	11507	1.20%	0.155%
89	14.544	4120	4122	4125	rBV	251	184	0.02%	0.002%
90	14.566	4125	4129	4132	rBV	249	257	0.03%	0.003%
91	14.634	4144	4150	4153	rBV2	369	430	0.04%	0.006%
92	14.675	4159	4163	4167	rBV2	326	347	0.04%	0.005%
93	14.711	4172	4174	4177	rBV2	331	243	0.03%	0.003%
94	14.878	4223	4226	4232	rVV3	340	311	0.03%	0.004%
95	15.074	4282	4287	4290	rBV2	352	344	0.04%	0.005%
96	15.351	4368	4373	4375	rBV	424	433	0.05%	0.006%
97	15.968	4562	4565	4568	rVB2	611	364	0.04%	0.005%
98	16.215	4640	4642	4646	rBV3	565	481	0.05%	0.006%
99	16.518	4733	4736	4737	rBV2	645	383	0.04%	0.005%
100	16.926	4859	4863	4865	rBV2	1057	1016	0.11%	0.014%




Sum of corrected areas: 7405954

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022124\
Data File : VU057914.D
Acq On : 21 Feb 2024 10:30
Operator : MD/SY
Sample : VU0221WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK042

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

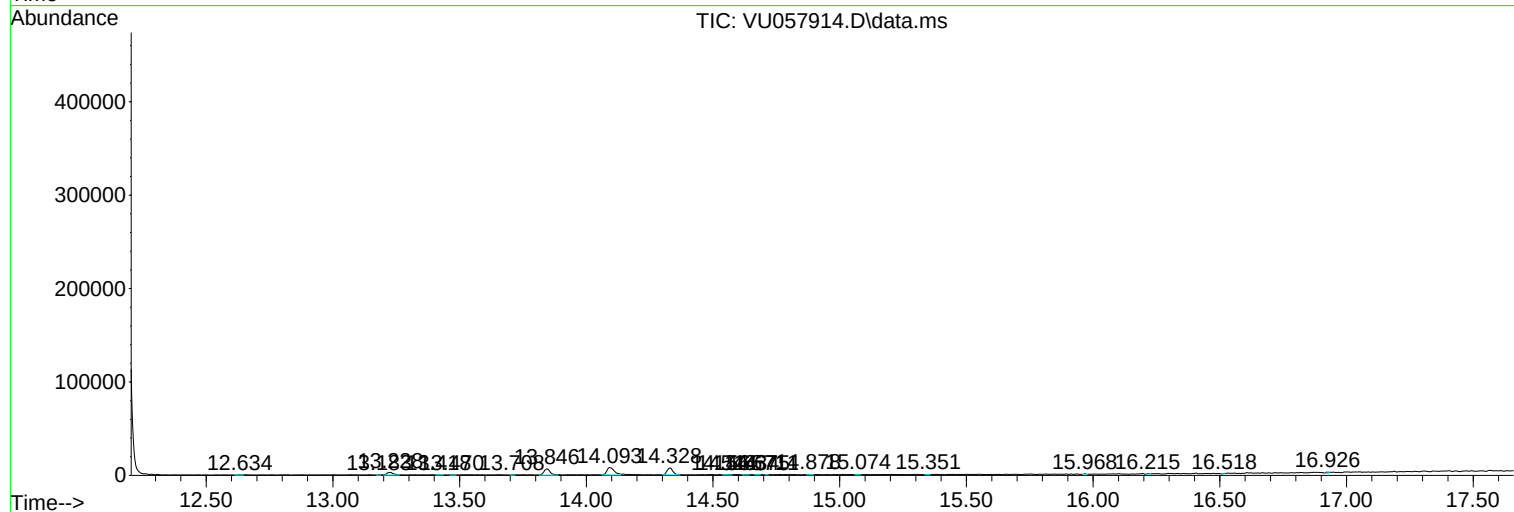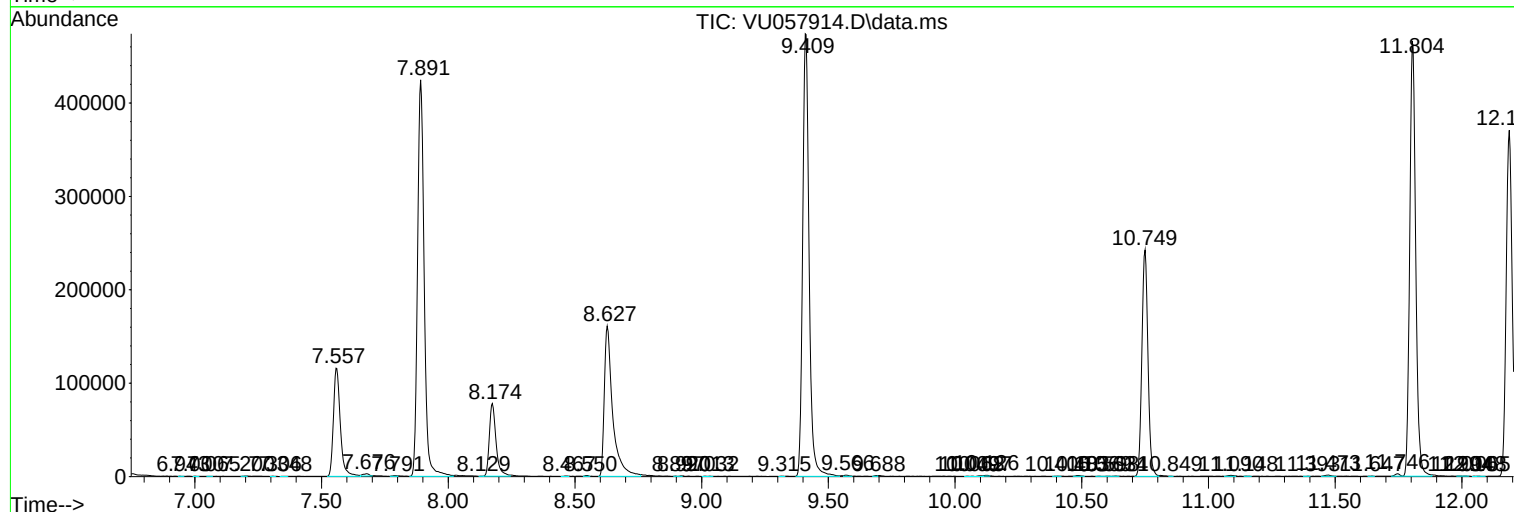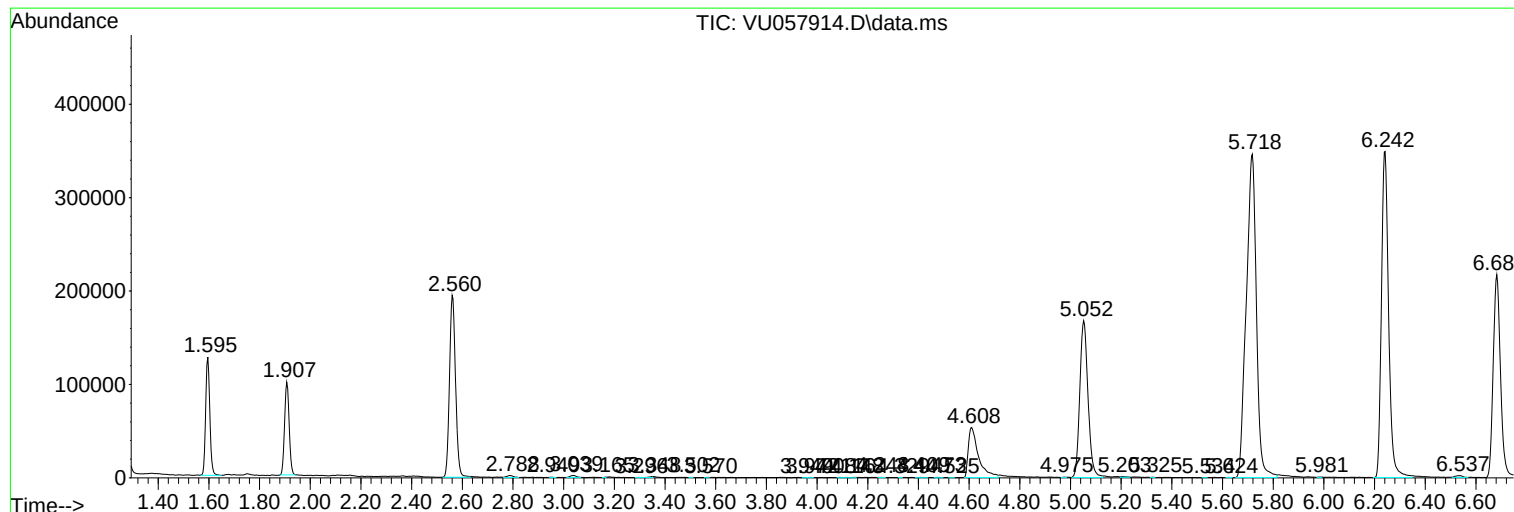

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022124\
Data File : VU057914.D
Acq On : 21 Feb 2024 10:30
Operator : MD/SY
Sample : VU0221WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK042

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022124\
Data File : VU057914.D
Acq On : 21 Feb 2024 10:30
Operator : MD/SY
Sample : VU0221WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK042

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------