

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022124\
 Data File : VU057916.D
 Acq On : 21 Feb 2024 11:21
 Operator : MD/SY
 Sample : P1504-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

Signal : TIC: VU057916.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	108	rVB	116342	129144	14.01%	1.810%
2	1.907	183	192	207	rVB	93003	120103	13.03%	1.684%
3	2.560	382	395	415	rBV	181210	300041	32.56%	4.206%
4	2.785	458	465	469	rBV2	1195	1610	0.17%	0.023%
5	2.936	509	512	516	rBV	182	205	0.02%	0.003%
6	3.036	535	543	552	rBV3	2181	4007	0.43%	0.056%
7	3.174	576	586	596	rVB3	614	1537	0.17%	0.022%
8	3.348	630	640	655	rVB4	1300	2666	0.29%	0.037%
9	3.676	739	742	746	rVV	233	166	0.02%	0.002%
10	3.853	793	797	800	rBV	213	184	0.02%	0.003%
11	4.029	848	852	854	rBV	357	319	0.03%	0.004%
12	4.078	863	867	870	rBV	219	168	0.02%	0.002%
13	4.103	872	875	880	rVV2	262	264	0.03%	0.004%
14	4.158	884	892	902	rBV	271	510	0.06%	0.007%
15	4.245	915	919	922	rBV	156	153	0.02%	0.002%
16	4.348	946	951	953	rBV	244	261	0.03%	0.004%
17	4.438	974	979	984	rBV2	260	346	0.04%	0.005%
18	4.608	1023	1032	1063	rBV	55773	154480	16.76%	2.166%
19	4.943	1133	1136	1137	rBV	272	173	0.02%	0.002%
20	5.052	1154	1170	1197	rBV	159522	361869	39.27%	5.073%
21	5.203	1215	1217	1219	rBV3	332	206	0.02%	0.003%
22	5.299	1242	1247	1251	rBV3	270	270	0.03%	0.004%
23	5.322	1251	1254	1257	rVB2	512	310	0.03%	0.004%
24	5.377	1267	1271	1273	rBV2	316	206	0.02%	0.003%
25	5.714	1356	1376	1400	rBV2	337224	921606	100.00%	12.919%
26	6.119	1499	1502	1503	rBV	307	200	0.02%	0.003%
27	6.187	1517	1523	1525	rBV2	157	177	0.02%	0.002%
28	6.238	1526	1539	1567	rBV	335473	655431	71.12%	9.188%
29	6.524	1623	1628	1630	rBV4	841	842	0.09%	0.012%
30	6.589	1643	1648	1650	rBV	299	311	0.03%	0.004%
31	6.682	1663	1677	1707	rBV	208368	421877	45.78%	5.914%
32	6.856	1728	1731	1734	rVB	281	175	0.02%	0.002%
33	6.891	1739	1742	1746	rVB2	269	177	0.02%	0.002%
34	6.910	1746	1748	1752	rVB2	305	164	0.02%	0.002%
35	6.936	1752	1756	1758	rBV	269	239	0.03%	0.003%
36	7.132	1814	1817	1822	rBV2	220	256	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022124\
 Data File : VU057916.D
 Acq On : 21 Feb 2024 11:21
 Operator : MD/SY
 Sample : P1504-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

37	7.209	1835	1841	1846	rVB2	489	586	0.06%	0.008%
38	7.319	1871	1875	1879	rBV2	187	177	0.02%	0.002%
39	7.357	1883	1887	1890	rBV2	267	283	0.03%	0.004%
40	7.460	1911	1919	1927	rVB2	349	601	0.07%	0.008%
41	7.499	1927	1931	1935	rBV2	263	277	0.03%	0.004%
42	7.560	1935	1950	1980	rBV	114647	213202	23.13%	2.989%
43	7.711	1995	1997	1999	rBV3	382	193	0.02%	0.003%
44	7.891	2037	2053	2088	rBV	409731	729114	79.11%	10.221%
45	8.132	2124	2128	2130	rVB2	223	167	0.02%	0.002%
46	8.174	2130	2141	2176	rBV	76338	139873	15.18%	1.961%
47	8.344	2192	2194	2197	rVV2	448	272	0.03%	0.004%
48	8.373	2201	2203	2209	rVB2	239	230	0.02%	0.003%
49	8.467	2226	2232	2237	rBV2	416	500	0.05%	0.007%
50	8.553	2254	2259	2263	rVB3	326	395	0.04%	0.006%
51	8.585	2265	2269	2271	rBV	322	301	0.03%	0.004%
52	8.627	2271	2282	2322	rBV2	162888	376496	40.85%	5.278%
53	8.868	2355	2357	2360	rBV2	226	177	0.02%	0.002%
54	9.119	2431	2435	2438	rBV2	218	246	0.03%	0.003%
55	9.331	2497	2501	2503	rBV	295	276	0.03%	0.004%
56	9.409	2513	2525	2547	rBV	464055	800685	86.88%	11.224%
57	9.563	2570	2573	2576	rBV2	548	448	0.05%	0.006%
58	9.643	2593	2598	2600	rBV2	248	265	0.03%	0.004%
59	9.688	2608	2612	2614	rBV2	369	266	0.03%	0.004%
60	9.778	2631	2640	2643	rBV2	265	444	0.05%	0.006%
61	9.872	2664	2669	2672	rBV2	253	267	0.03%	0.004%
62	10.110	2740	2743	2746	rVV3	357	328	0.04%	0.005%
63	10.132	2748	2750	2752	rVV	486	250	0.03%	0.004%
64	10.225	2776	2779	2782	rVV2	199	178	0.02%	0.002%
65	10.312	2800	2806	2811	rBV	273	332	0.04%	0.005%
66	10.479	2855	2858	2865	rBV2	371	441	0.05%	0.006%
67	10.749	2929	2942	2961	rBV	243951	403780	43.81%	5.660%
68	11.019	3022	3026	3029	rVV2	172	190	0.02%	0.003%
69	11.206	3079	3084	3088	rBV2	263	249	0.03%	0.003%
70	11.380	3131	3138	3140	rBV2	256	274	0.03%	0.004%
71	11.437	3153	3156	3162	rBV2	207	239	0.03%	0.003%
72	11.470	3162	3166	3170	rBV2	549	614	0.07%	0.009%
73	11.595	3201	3205	3210	rVB	312	309	0.03%	0.004%
74	11.682	3227	3232	3235	rVB2	194	178	0.02%	0.002%
75	11.720	3241	3244	3246	rBV	267	156	0.02%	0.002%
76	11.743	3247	3251	3259	rBB3	1343	1276	0.14%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022124\
 Data File : VU057916.D
 Acq On : 21 Feb 2024 11:21
 Operator : MD/SY
 Sample : P1504-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

77	11.804	3259	3270	3291	rBV	458832	758327	82.28%	10.631%
78	12.026	3334	3339	3343	rBV3	434	506	0.05%	0.007%
79	12.187	3370	3389	3416	rBV	357731	608314	66.01%	8.528%
80	12.354	3438	3441	3447	rBV2	247	233	0.03%	0.003%
81	12.383	3447	3450	3455	rVV2	153	181	0.02%	0.003%
82	12.415	3456	3460	3465	rVB2	372	328	0.04%	0.005%
83	12.444	3465	3469	3476	rVB2	294	374	0.04%	0.005%
84	12.872	3599	3602	3607	rBV	244	209	0.02%	0.003%
85	13.048	3652	3657	3659	rBV	302	291	0.03%	0.004%
86	13.228	3709	3713	3715	rBV3	582	515	0.06%	0.007%
87	13.579	3819	3822	3826	rBV	249	205	0.02%	0.003%
88	13.637	3836	3840	3848	rVB2	392	536	0.06%	0.008%
89	13.682	3848	3854	3857	rBV	207	274	0.03%	0.004%
90	13.852	3901	3907	3917	rVB5	1600	2637	0.29%	0.037%
91	13.894	3918	3920	3927	rBV2	286	296	0.03%	0.004%
92	13.952	3934	3938	3941	rBV2	201	163	0.02%	0.002%
93	14.106	3979	3986	3990	rBV3	1136	1439	0.16%	0.020%
94	14.280	4037	4040	4043	rBV2	330	302	0.03%	0.004%
95	14.338	4051	4058	4064	rBV4	1186	1784	0.19%	0.025%
96	14.473	4095	4100	4103	rBV3	308	282	0.03%	0.004%
97	14.669	4156	4161	4163	rBV	237	229	0.02%	0.003%
98	14.797	4198	4201	4204	rBV2	341	320	0.03%	0.004%
99	15.672	4471	4473	4479	rBV2	343	232	0.03%	0.003%
100	16.113	4607	4610	4612	rBV2	445	320	0.03%	0.004%




Sum of corrected areas: 7133485

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022124\
Data File : VU057916.D
Acq On : 21 Feb 2024 11:21
Operator : MD/SY
Sample : P1504-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

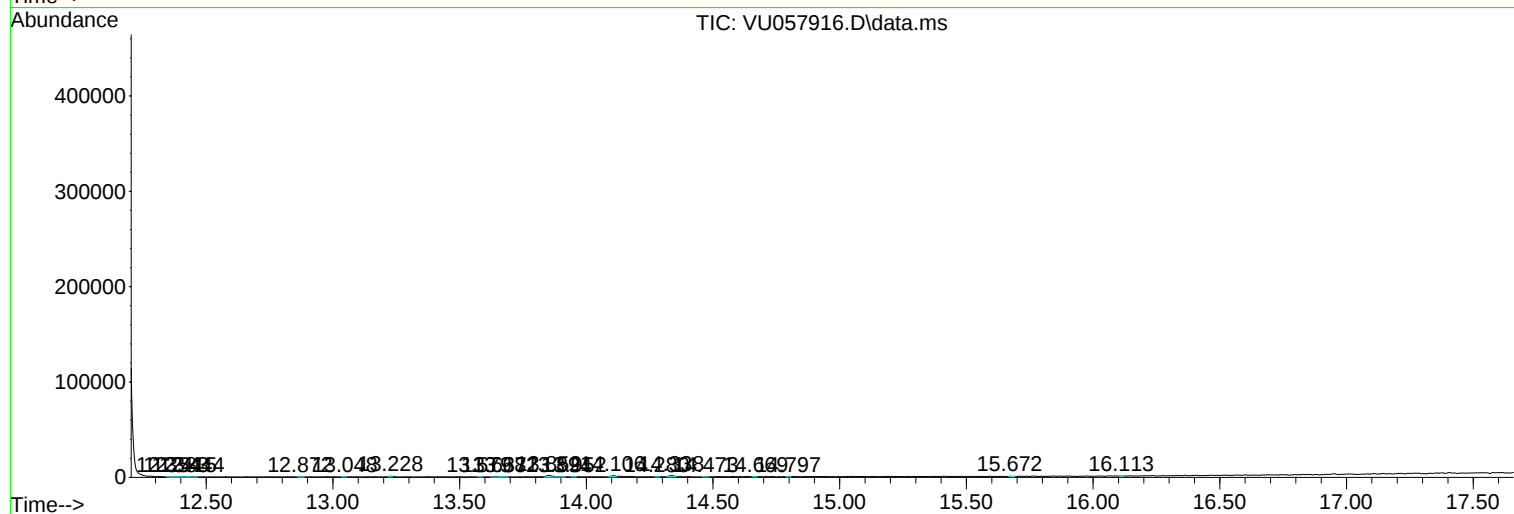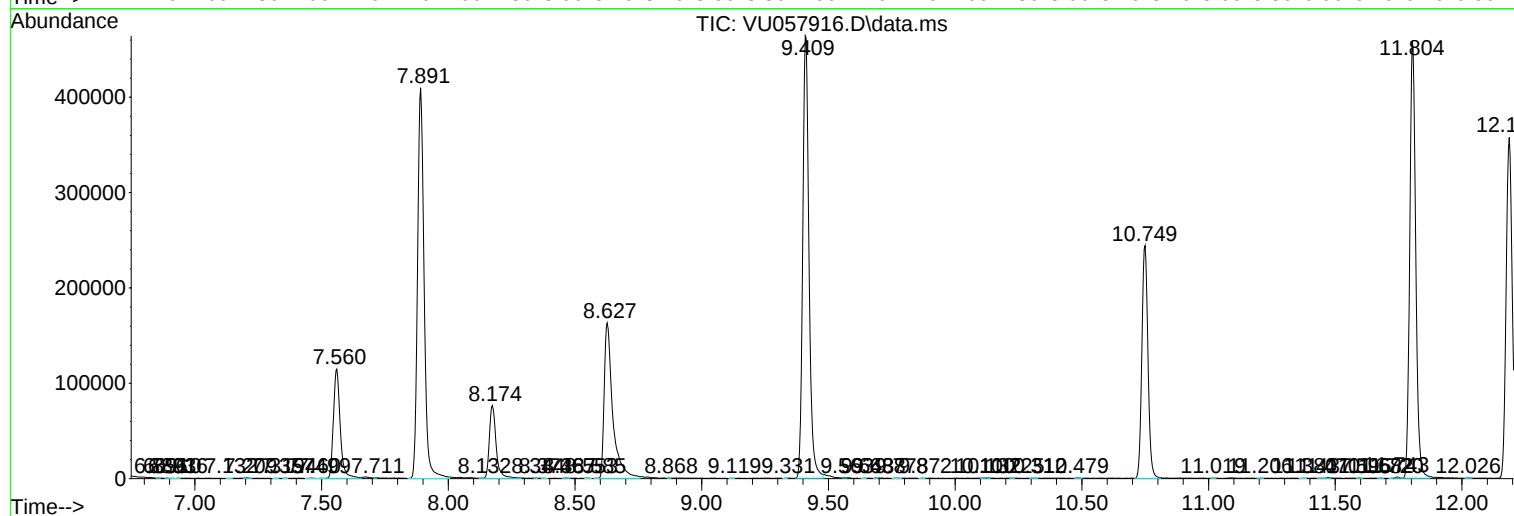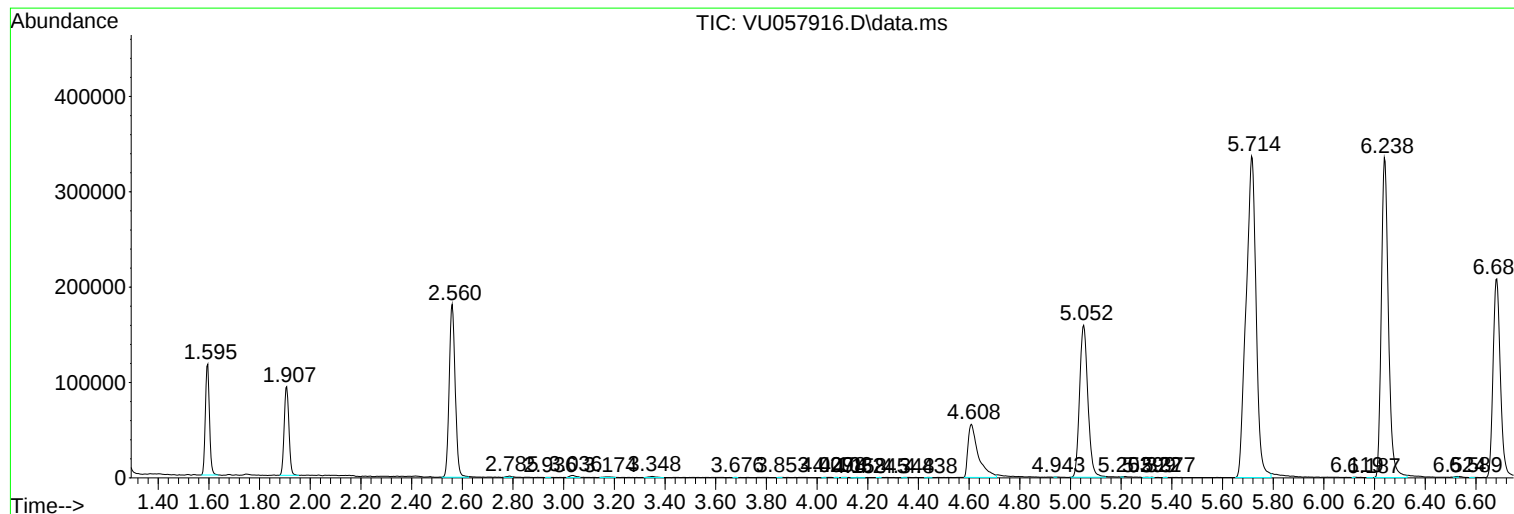

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022124\
Data File : VU057916.D
Acq On : 21 Feb 2024 11:21
Operator : MD/SY
Sample : P1504-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022124\
Data File : VU057916.D
Acq On : 21 Feb 2024 11:21
Operator : MD/SY
Sample : P1504-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------