


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022124\
Data File : VU057912.D
Acq On : 21 Feb 2024 09:07
Operator : MD/SY
Sample : BFB041
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB041

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Title : VOC Analysis
Last Update : Wed Feb 21 23:55:33 2024

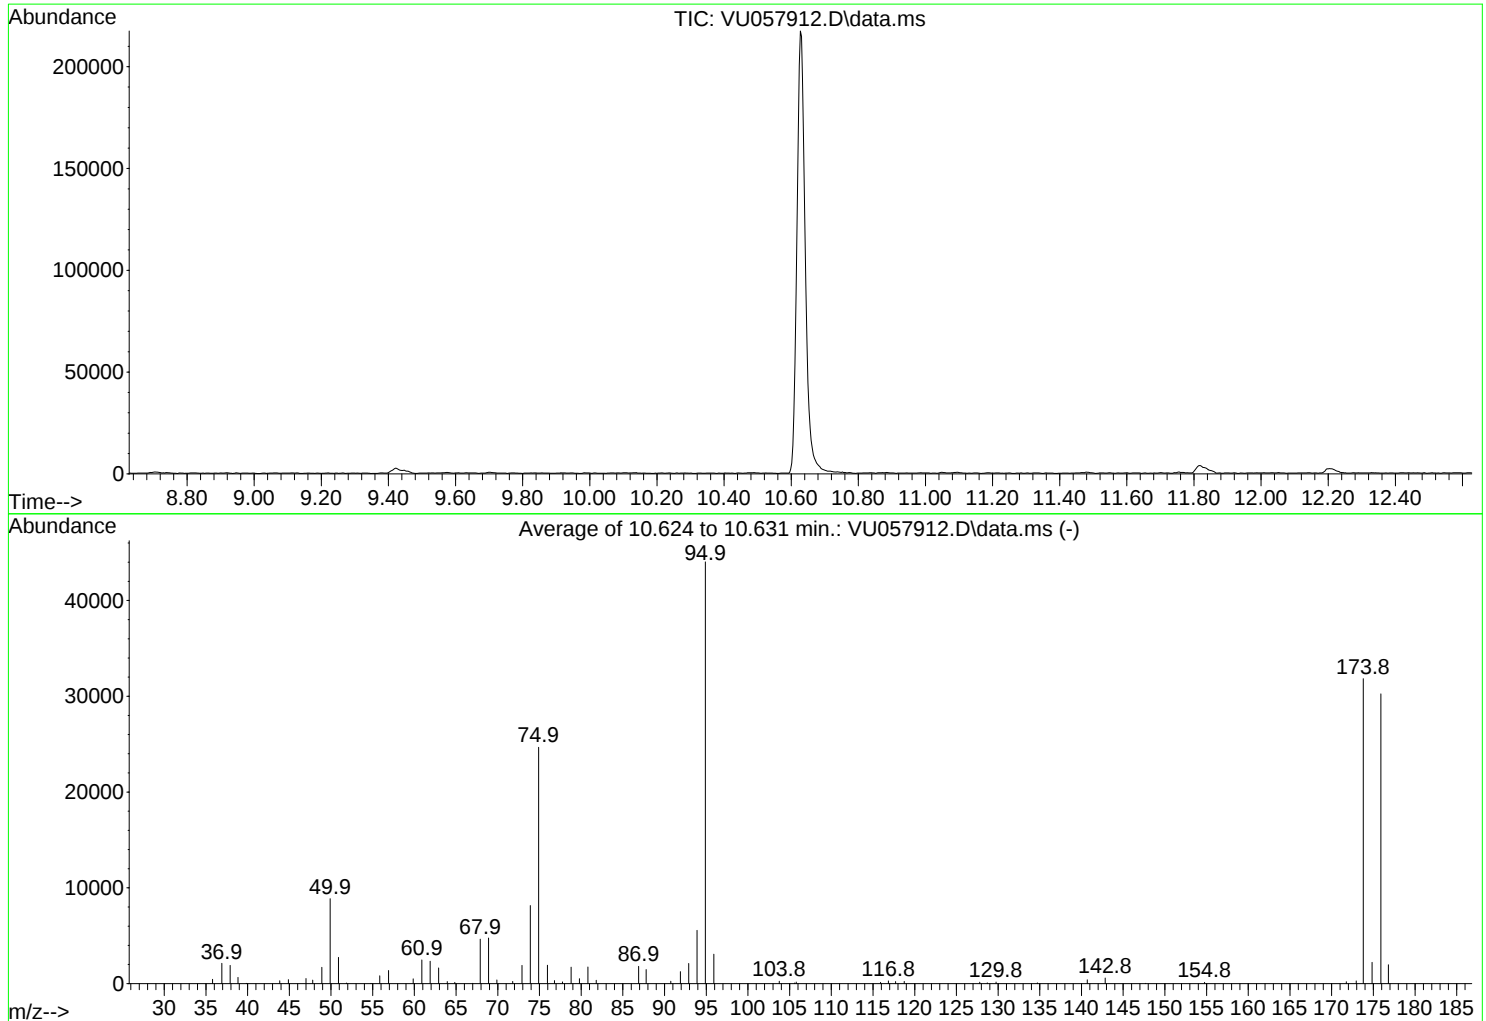

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.1	8863	PASS
75	95	30	80	56.0	24680	PASS
95	95	100	100	100.0	44035	PASS
96	95	5	9	7.0	3076	PASS
173	174	0.00	2	0.9	291	PASS
174	95	50	120	72.3	31832	PASS
175	174	5	9	7.0	2226	PASS
176	174	95	101	95.0	30245	PASS
177	176	5	9	6.5	1966	PASS

Scan 2892 (10.589 min): VU057912.D\data.ms
BFB041

m/z	Abundance
39.90	107.0
43.80	260.0

Instrument :
MSVOA_U
ClientSampleId :
BFB041

m/z	Abundance
35.80	470.0
36.90	1979.0
37.90	1902.0
38.80	602.0
39.80	119.0
43.90	551.0
44.90	382.0
47.00	598.0
47.80	344.0
48.90	1591.0
49.90	8471.0
50.90	2729.0
51.80	115.0
54.80	113.0
55.90	827.0
56.90	1253.0
59.80	499.0
60.90	2543.0
61.90	2255.0
62.90	1554.0
64.00	225.0
64.80	134.0
67.90	4332.0
68.90	4546.0
69.90	384.0
71.80	234.0
72.90	1820.0
73.90	7804.0
74.90	23600.0
76.00	1880.0
76.80	301.0
77.80	222.0
78.80	1676.0
79.80	472.0
80.80	1545.0
81.80	368.0
86.90	1700.0
87.80	1364.0
90.80	267.0
91.90	1213.0
92.90	1912.0
93.90	5485.0
94.90	41864.0
95.90	2961.0
103.80	226.0
105.60	213.0
115.90	128.0
116.80	325.0
117.70	204.0
118.70	251.0
127.80	114.0
128.70	114.0
129.70	140.0
140.70	362.0
142.80	491.0
154.80	139.0
171.70	174.0
172.90	265.0
173.80	29952.0
174.80	2153.0
175.90	28232.0
176.80	1878.0

Instrument :
MSVOA_U
ClientSampleId :
BFB041

m/z	Abundance
35.80	460.0
36.90	2187.0
37.90	1908.0
38.80	677.0
39.80	139.0
43.90	565.0
44.90	451.0
47.00	539.0
47.80	398.0
48.90	1792.0
49.90	9167.0
50.90	2831.0
51.90	104.0
55.80	850.0
56.90	1427.0
59.80	513.0
60.90	2580.0
61.90	2395.0
62.90	1689.0
64.00	226.0
64.80	147.0
67.00	104.0
67.90	4746.0
68.90	4827.0
69.90	388.0
71.80	239.0
72.90	1965.0
73.90	8461.0
74.90	25392.0
75.90	1971.0
76.80	351.0
77.80	176.0
78.80	1764.0
79.80	531.0
80.80	1779.0
81.80	357.0
86.90	1863.0
87.80	1482.0
90.70	263.0
91.90	1261.0
92.90	2186.0
93.90	5775.0
94.90	45472.0
95.90	3162.0
103.80	255.0
105.80	227.0
115.90	152.0
116.90	284.0
117.70	236.0
118.80	245.0
127.80	155.0
128.70	119.0
129.70	167.0
134.70	110.0
140.70	399.0
142.90	604.0
154.80	135.0
171.70	211.0
173.00	292.0
173.80	32824.0
174.80	2275.0
175.90	31208.0
176.80	2022.0

Instrument :
MSVOA_U
ClientSampleId :
BFB041

m/z	Abundance
35.80	427.0
36.90	2192.0
37.90	1895.0
38.90	693.0
39.90	166.0
43.90	546.0
44.90	419.0
47.00	489.0
47.80	349.0
48.90	1734.0
49.90	8950.0
50.90	2657.0
55.80	802.0
56.90	1434.0
59.90	475.0
60.90	2298.0
61.90	2375.0
62.90	1658.0
63.90	231.0
64.90	134.0
67.90	4849.0
68.90	4896.0
69.90	371.0
71.80	241.0
72.90	1949.0
73.90	8215.0
74.90	25048.0
75.90	1925.0
76.80	329.0
77.70	162.0
78.80	1736.0
79.80	538.0
80.80	1903.0
81.80	327.0
86.90	1875.0
87.80	1553.0
90.70	213.0
91.90	1278.0
92.90	2236.0
93.90	5442.0
94.90	44768.0
95.90	3104.0
103.70	251.0
105.80	254.0
115.90	149.0
116.80	224.0
117.70	224.0
118.80	234.0
127.80	173.0
129.80	189.0
134.70	132.0
140.70	424.0
142.90	656.0
147.70	103.0
154.70	128.0
171.80	224.0
172.90	317.0
173.80	32720.0
174.90	2251.0
175.90	31296.0
176.80	1999.0

Instrument :
MSVOA_U
ClientSampleId :
BFB041