
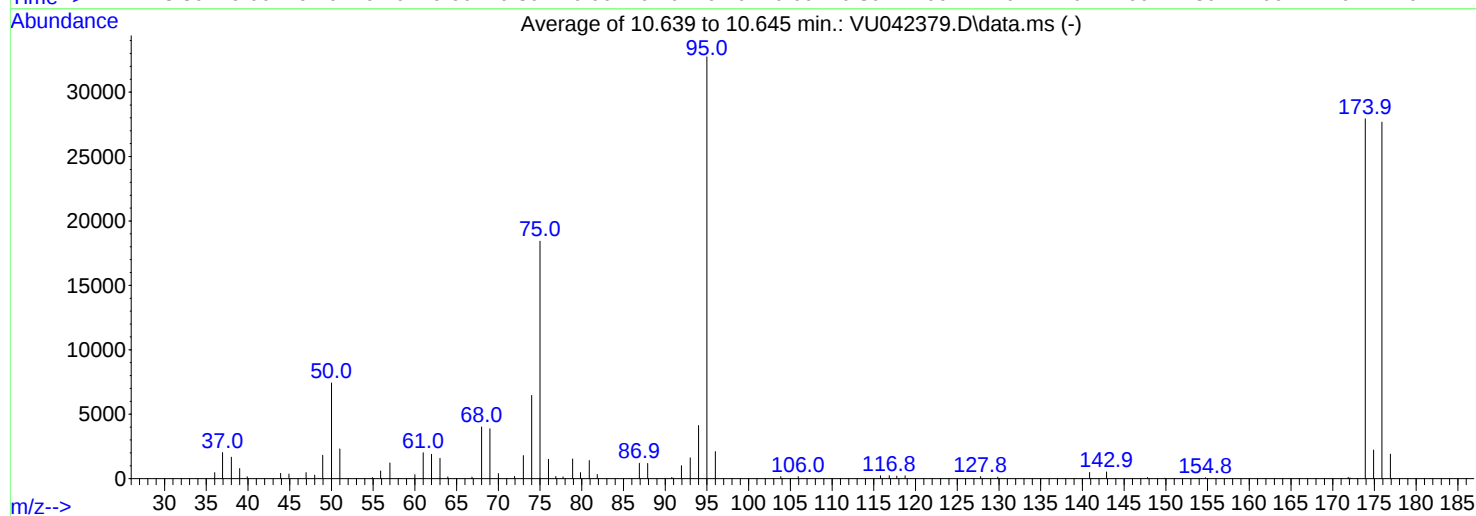


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022221\
Data File : VU042379.D
Acq On : 22 Feb 2021 09:01
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U021721W.M
Title : SW846 8260
Last Update : Fri Feb 19 02:55:52 2021

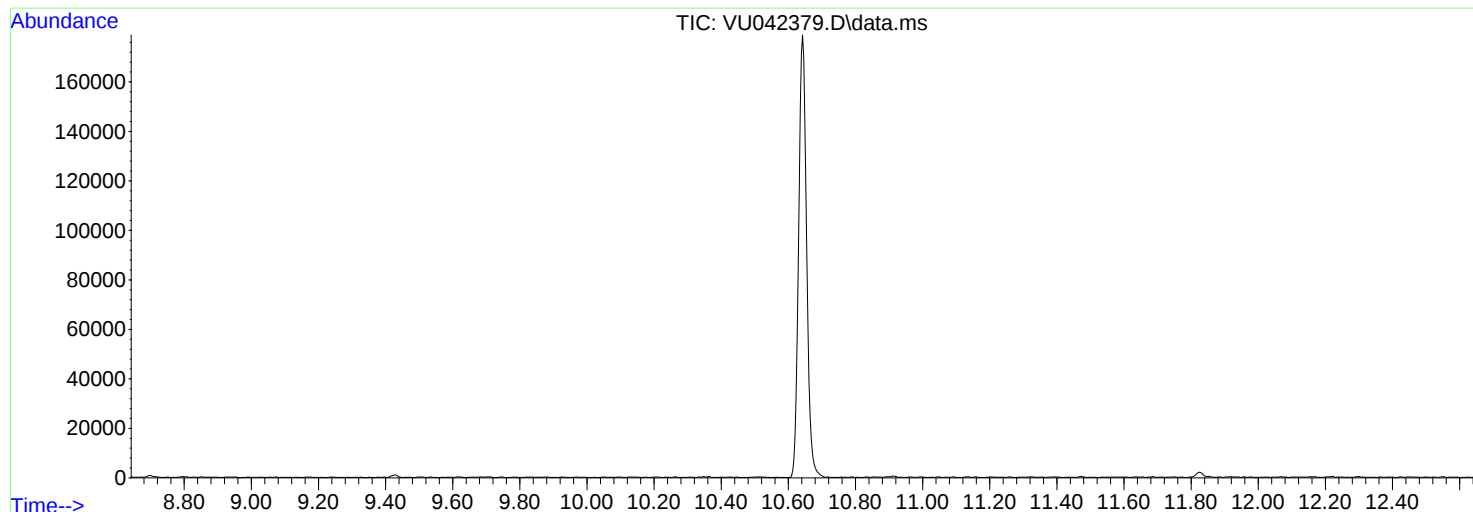

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2880

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	7428	PASS
75	95	30	60	56.3	18435	PASS
95	95	100	100	100.0	32739	PASS
96	95	5	9	6.4	2095	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.3	27928	PASS
175	174	5	9	8.0	2223	PASS
176	174	95	101	99.1	27669	PASS
177	176	5	9	6.9	1902	PASS