

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022222\
 Data File : VU047232.D
 Acq On : 22 Feb 2022 15:21
 Operator : SY/MD
 Sample : VU0222WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK069

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

Signal : TIC: VU047232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	105	rVB	213096	258196	15.79%	1.961%
2	1.919	172	180	202	rBV	169291	232984	14.24%	1.769%
3	2.571	371	383	419	rBV	369068	623859	38.14%	4.737%
4	2.780	441	448	450	rBV4	629	639	0.04%	0.005%
5	2.887	477	481	485	rVB3	391	291	0.02%	0.002%
6	2.941	495	498	500	rBV	256	182	0.01%	0.001%
7	2.957	500	503	504	rBV2	291	170	0.01%	0.001%
8	3.051	526	532	541	rBV5	979	1850	0.11%	0.014%
9	3.102	543	548	556	rVB4	473	645	0.04%	0.005%
10	3.179	565	572	573	rBV	1031	835	0.05%	0.006%
11	3.282	600	604	608	rVB2	285	169	0.01%	0.001%
12	3.321	612	616	620	rBV2	254	204	0.01%	0.002%
13	3.359	625	628	630	rVV3	447	309	0.02%	0.002%
14	3.427	647	649	653	rVB	332	228	0.01%	0.002%
15	3.449	653	656	663	rBV2	145	195	0.01%	0.001%
16	3.520	671	678	681	rBV3	186	204	0.01%	0.002%
17	3.768	751	755	759	rBV3	194	163	0.01%	0.001%
18	3.787	759	761	767	rVB3	251	205	0.01%	0.002%
19	3.851	778	781	786	rBV2	217	180	0.01%	0.001%
20	3.890	790	793	799	rBV3	225	176	0.01%	0.001%
21	4.044	838	841	845	rVV3	277	161	0.01%	0.001%
22	4.121	862	865	870	rVB2	220	164	0.01%	0.001%
23	4.150	870	874	877	rBV2	269	240	0.01%	0.002%
24	4.308	917	923	926	rBV2	205	178	0.01%	0.001%
25	4.530	986	992	995	rBV3	255	265	0.02%	0.002%
26	4.571	1000	1005	1008	rBV2	316	285	0.02%	0.002%
27	4.636	1008	1025	1058	rBV	166977	464074	28.37%	3.524%
28	4.919	1111	1113	1117	rVB	247	158	0.01%	0.001%
29	4.980	1129	1132	1135	rBV	284	218	0.01%	0.002%
30	5.070	1142	1160	1185	rBV	287781	631976	38.64%	4.799%
31	5.279	1222	1225	1227	rBV	329	220	0.01%	0.002%
32	5.391	1258	1260	1267	rVB	426	381	0.02%	0.003%
33	5.427	1267	1271	1275	rBV3	319	327	0.02%	0.002%
34	5.452	1275	1279	1287	rVB2	223	269	0.02%	0.002%
35	5.494	1287	1292	1294	rBV2	224	192	0.01%	0.001%
36	5.578	1310	1318	1323	rBV3	399	633	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022222\
 Data File : VU047232.D
 Acq On : 22 Feb 2022 15:21
 Operator : SY/MD
 Sample : VU0222WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK069

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	5.629	1329	1334	1338	rBV2	272	239	0.01%	0.002%
38	5.729	1342	1365	1389	rBV2	614514	1635691	100.00%	12.420%
39	5.938	1427	1430	1432	rBV2	325	245	0.01%	0.002%
40	6.108	1478	1483	1485	rBV2	368	310	0.02%	0.002%
41	6.137	1490	1492	1497	rVB2	456	324	0.02%	0.002%
42	6.176	1502	1504	1509	rVB3	226	167	0.01%	0.001%
43	6.253	1513	1528	1546	rBV	453813	845548	51.69%	6.420%
44	6.388	1567	1570	1575	rVB3	347	320	0.02%	0.002%
45	6.430	1581	1583	1589	rVB3	300	182	0.01%	0.001%
46	6.533	1606	1615	1624	rBV6	1614	3008	0.18%	0.023%
47	6.575	1624	1628	1631	rBV2	237	199	0.01%	0.002%
48	6.597	1631	1635	1638	rVB2	377	274	0.02%	0.002%
49	6.693	1650	1665	1688	rBV	373013	725282	44.34%	5.507%
50	6.809	1694	1701	1708	rBV4	1095	1497	0.09%	0.011%
51	6.861	1713	1717	1718	rBV2	294	198	0.01%	0.002%
52	6.870	1718	1720	1723	rVB3	378	177	0.01%	0.001%
53	6.915	1731	1734	1740	rBV3	183	170	0.01%	0.001%
54	6.947	1740	1744	1747	rBV2	227	161	0.01%	0.001%
55	7.044	1765	1774	1780	rBV4	1183	1823	0.11%	0.014%
56	7.073	1780	1783	1786	rVB	519	403	0.02%	0.003%
57	7.092	1786	1789	1793	rVB4	236	195	0.01%	0.001%
58	7.131	1793	1801	1803	rVB4	342	353	0.02%	0.003%
59	7.182	1809	1817	1828	rBV3	1906	3405	0.21%	0.026%
60	7.272	1843	1845	1850	rVB3	375	264	0.02%	0.002%
61	7.320	1857	1860	1861	rBV2	323	167	0.01%	0.001%
62	7.388	1876	1881	1885	rBV2	217	229	0.01%	0.002%
63	7.449	1897	1900	1903	rVB3	229	175	0.01%	0.001%
64	7.475	1905	1908	1913	rVB3	272	256	0.02%	0.002%
65	7.501	1913	1916	1922	rBV3	284	280	0.02%	0.002%
66	7.568	1924	1937	1955	rBV	239174	406197	24.83%	3.084%
67	7.684	1965	1973	1983	rVB3	1860	2843	0.17%	0.022%
68	7.774	1996	2001	2002	rBV3	251	207	0.01%	0.002%
69	7.796	2004	2008	2012	rVV3	390	414	0.03%	0.003%
70	7.899	2025	2040	2056	rVV	830094	1406099	85.96%	10.677%
71	7.970	2056	2062	2075	rVB	11325	19793	1.21%	0.150%
72	8.070	2090	2093	2103	rVB4	473	592	0.04%	0.004%
73	8.182	2114	2128	2144	rBV	161740	274690	16.79%	2.086%
74	8.475	2207	2219	2231	rBV2	21031	37214	2.28%	0.283%
75	8.574	2247	2250	2252	rBV2	353	239	0.01%	0.002%
76	8.636	2256	2269	2296	rBV	634827	1052931	64.37%	7.995%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022222\
 Data File : VU047232.D
 Acq On : 22 Feb 2022 15:21
 Operator : SY/MD
 Sample : VU0222WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK069

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

77	8.771	2308	2311	2312	rBV	268	181	0.01%	0.001%
78	8.809	2320	2323	2326	rVB2	463	354	0.02%	0.003%
79	8.832	2326	2330	2331	rBV2	345	222	0.01%	0.002%
80	8.922	2349	2358	2367	rBV4	997	1859	0.11%	0.014%
81	8.992	2377	2380	2383	rBV3	512	345	0.02%	0.003%
82	9.028	2388	2391	2395	rBV3	279	264	0.02%	0.002%
83	9.082	2405	2408	2412	rBV4	297	275	0.02%	0.002%
84	9.137	2415	2425	2428	rBV3	2392	4414	0.27%	0.034%
85	9.420	2500	2513	2531	rBV	650211	1053082	64.38%	7.996%
86	10.674	2895	2903	2914	rVB3	8723	13340	0.82%	0.101%
87	10.758	2917	2929	2948	rVV	536924	854823	52.26%	6.491%
88	10.896	2963	2972	2990	rVB	22432	40587	2.48%	0.308%
89	11.462	3140	3148	3161	rVB4	7010	11841	0.72%	0.090%
90	11.581	3180	3185	3194	rVB5	1658	2366	0.14%	0.018%
91	11.693	3214	3220	3229	rBV4	3868	5806	0.35%	0.044%
92	11.748	3234	3237	3240	rBV3	784	450	0.03%	0.003%
93	11.812	3244	3257	3270	rBV	779710	1207603	73.83%	9.170%
94	11.944	3292	3298	3302	rBV4	2747	3583	0.22%	0.027%
95	12.195	3360	3376	3390	rBV	808567	1291866	78.98%	9.810%
96	12.330	3413	3418	3427	rVB5	2527	3701	0.23%	0.028%
97	12.774	3547	3556	3569	rBV2	12949	20828	1.27%	0.158%
98	13.848	3883	3890	3894	rVB6	1744	2237	0.14%	0.017%
99	14.089	3961	3965	3973	rVB2	2548	3178	0.19%	0.024%
100	14.336	4036	4042	4048	rVB5	1956	2125	0.13%	0.016%




Sum of corrected areas: 13169516

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022222\
Data File : VU047232.D
Acq On : 22 Feb 2022 15:21
Operator : SY/MD
Sample : VU0222WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK069

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

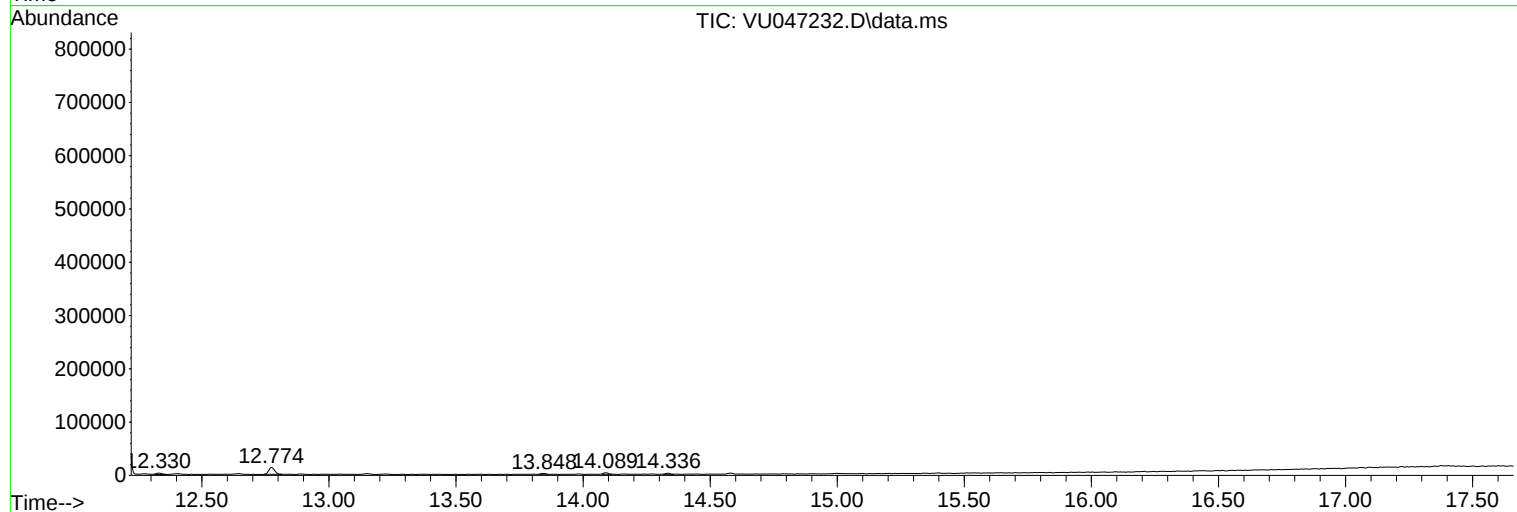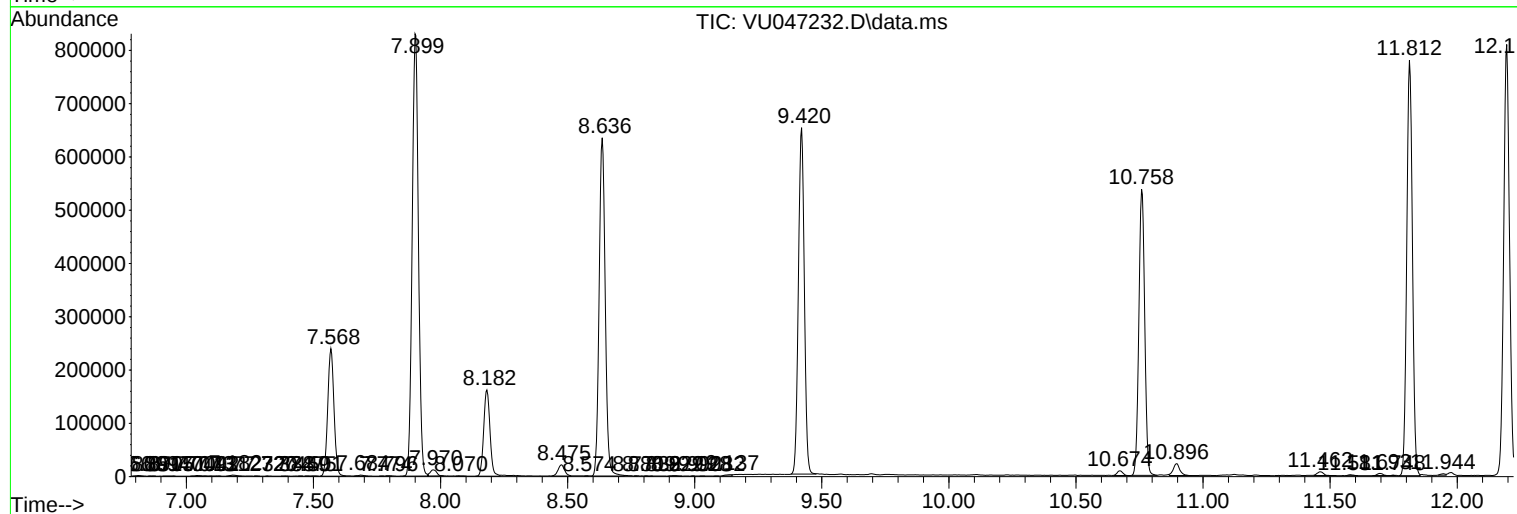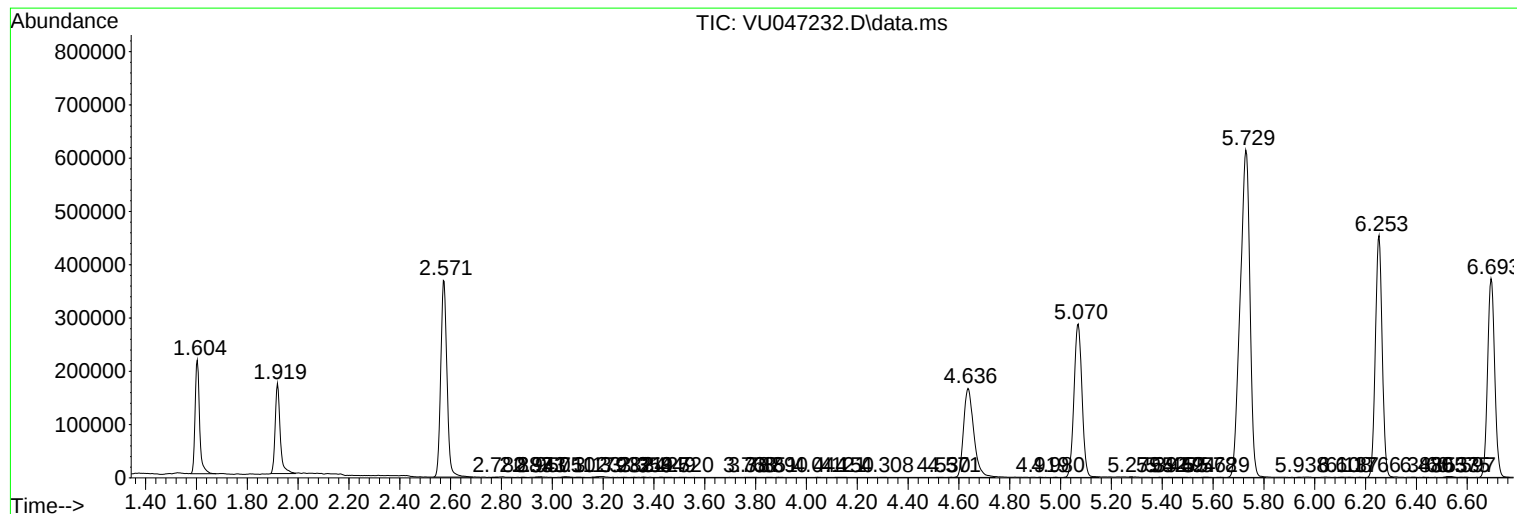

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022222\
Data File : VU047232.D
Acq On : 22 Feb 2022 15:21
Operator : SY/MD
Sample : VU0222WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK069

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022222\
Data File : VU047232.D
Acq On : 22 Feb 2022 15:21
Operator : SY/MD
Sample : VU0222WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK069

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------