


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022222\
Data File : VU047230.D
Acq On : 22 Feb 2022 13:17
Operator : SY/MD
Sample : BFB046
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB046

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Title : VOC Analysis
Last Update : Fri Feb 18 00:54:38 2022

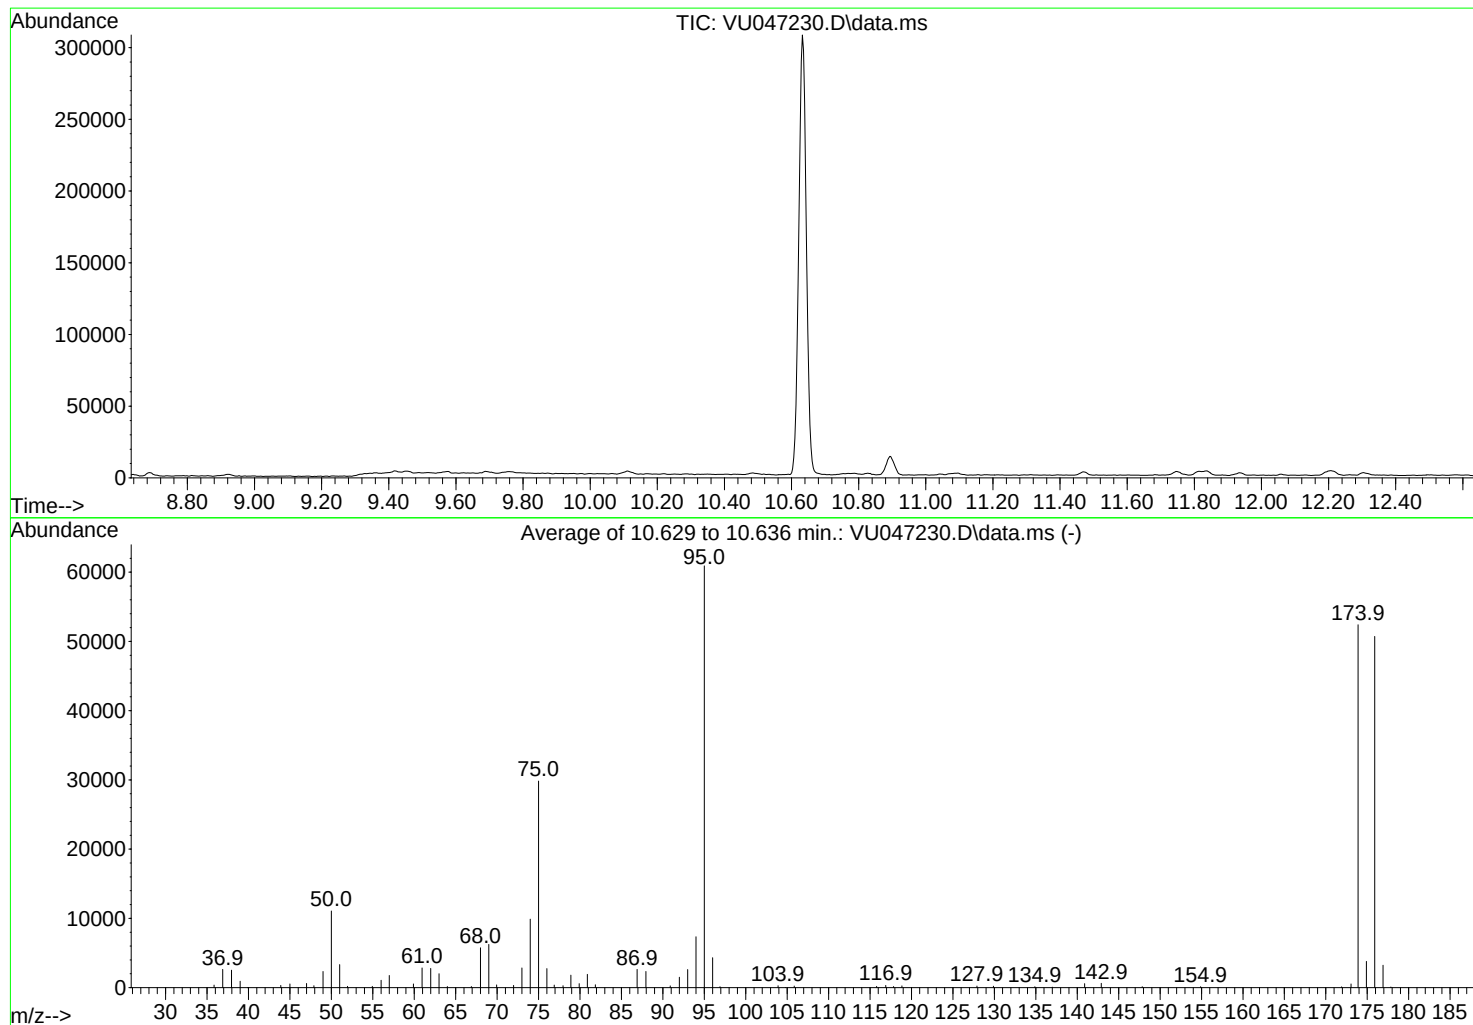

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	11058	PASS
75	95	30	80	49.0	29827	PASS
95	95	100	100	100.0	60912	PASS
96	95	5	9	7.1	4330	PASS
173	174	0.00	2	1.0	525	PASS
174	95	50	120	86.0	52408	PASS
175	174	5	9	7.2	3781	PASS
176	174	95	101	96.8	50715	PASS
177	176	5	9	6.4	3245	PASS

m/z	Abundance
35.90	1188.0
37.90	391.0
39.00	103.0
39.90	230.0
43.90	407.0
206.90	209.0

Instrument :
MSVOA_U
ClientSampleId :
BFB046

m/z	Abundance
35.90	1552.0
36.90	2751.0
38.00	2909.0
39.00	1011.0
39.90	229.0
43.90	688.0
45.00	516.0
47.00	644.0
47.90	278.0
49.00	2352.0
50.00	11054.0
51.00	3372.0
52.00	173.0
54.90	191.0
56.00	1080.0
57.00	1745.0
59.90	501.0
60.90	2809.0
62.00	2779.0
63.00	1948.0
64.00	158.0
66.90	135.0
68.00	5751.0
69.00	6104.0
69.90	377.0
72.00	307.0
73.00	2825.0
74.00	9771.0
75.00	29624.0
76.00	2807.0
76.90	384.0
78.00	256.0
78.90	1750.0
79.90	512.0
80.90	1888.0
81.80	397.0
86.90	2546.0
87.90	2325.0
90.90	244.0
92.00	1584.0
93.00	2489.0
94.00	7180.0
95.00	58840.0
96.00	4178.0
96.90	126.0
103.90	247.0
105.90	241.0
115.80	189.0
116.90	332.0
117.80	163.0
118.80	259.0
127.90	171.0
129.90	209.0
134.90	118.0
140.90	552.0
142.90	572.0
147.80	152.0
154.90	150.0
171.90	110.0
173.00	467.0
173.90	50296.0
174.90	3725.0
175.90	47832.0
176.90	3174.0
177.80	101.0
207.00	205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB046

m/z	Abundance
35.90	1575.0
36.90	2662.0
38.00	2980.0
39.00	1094.0
40.00	223.0
44.00	741.0
45.00	542.0
47.00	618.0
47.90	282.0
49.00	2446.0
50.00	11411.0
51.00	3437.0
52.00	183.0
54.90	186.0
56.00	1104.0
57.00	1807.0
59.90	541.0
61.00	2966.0
62.00	2858.0
63.00	2073.0
64.00	169.0
66.90	156.0
68.00	5930.0
69.00	6486.0
70.00	410.0
72.00	352.0
73.00	2929.0
74.00	10138.0
75.00	30680.0
76.00	2827.0
76.90	370.0
77.90	292.0
78.90	1877.0
79.90	589.0
80.90	1995.0
81.80	419.0
86.90	2721.0
87.90	2370.0
90.90	262.0
92.00	1537.0
93.00	2720.0
94.00	7601.0
95.00	62960.0
96.00	4542.0
96.90	161.0
103.90	290.0
105.80	243.0
115.80	202.0
116.90	336.0
117.90	173.0
118.80	262.0
127.90	228.0
129.90	212.0
134.90	147.0
137.00	106.0
140.90	591.0
142.90	647.0
147.80	138.0
154.90	159.0
171.90	138.0
173.00	535.0
173.90	54088.0
174.90	3851.0
175.90	52544.0
176.90	3363.0
177.90	103.0
207.00	191.0

Instrument :
MSVOA_U
ClientSampleId :
BFB046

m/z	Abundance
35.90	1572.0
36.90	2465.0
38.00	2875.0
39.00	1014.0
40.00	248.0
43.90	758.0
45.00	510.0
47.00	559.0
47.90	254.0
49.00	2220.0
50.00	10709.0
51.00	3196.0
51.90	180.0
55.00	185.0
56.00	984.0
57.00	1685.0
59.90	551.0
61.00	2738.0
62.00	2697.0
63.00	2019.0
64.00	150.0
66.90	177.0
68.00	5610.0
69.00	6152.0
70.00	404.0
72.00	342.0
73.00	2742.0
74.00	9731.0
75.00	29176.0
76.00	2638.0
76.90	343.0
77.90	268.0
78.90	1797.0
79.90	606.0
80.90	1905.0
81.90	428.0
86.90	2626.0
88.00	2295.0
90.90	244.0
92.00	1405.0
93.00	2609.0
94.00	7291.0
95.00	60936.0
96.00	4271.0
96.90	159.0
103.90	288.0
104.80	100.0
105.80	220.0
115.80	200.0
116.90	312.0
117.90	169.0
118.90	251.0
127.90	269.0
129.90	211.0
134.90	148.0
137.00	117.0
140.90	573.0
142.90	640.0
147.90	139.0
154.90	137.0
171.90	130.0
173.10	572.0
173.90	52840.0
174.90	3768.0
175.90	51768.0
176.90	3199.0
177.90	101.0
206.90	176.0

Instrument :
MSVOA_U
ClientSampleId :
BFB046