

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
 Data File : VU057920.D
 Acq On : 22 Feb 2024 10:51
 Operator : MD/SY
 Sample : VU0222WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK043

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

Signal : TIC: VU057920.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	114	rVB	125562	140683	14.72%	1.902%
2	1.907	184	192	206	rVB	100735	129121	13.51%	1.746%
3	2.560	383	395	415	rBV	194499	322114	33.69%	4.356%
4	2.718	441	444	448	rVB	333	229	0.02%	0.003%
5	2.788	460	466	476	rVB2	2304	3486	0.36%	0.047%
6	2.827	476	478	481	rBV	283	222	0.02%	0.003%
7	3.039	535	544	553	rBV2	2229	3402	0.36%	0.046%
8	3.139	572	575	580	rVB	263	197	0.02%	0.003%
9	3.165	580	583	590	rBV3	596	814	0.09%	0.011%
10	3.251	603	610	617	rBV2	271	549	0.06%	0.007%
11	3.354	634	642	647	rVV4	1024	1483	0.16%	0.020%
12	3.544	698	701	705	rVB2	299	255	0.03%	0.003%
13	3.570	705	709	711	rBV2	275	252	0.03%	0.003%
14	3.785	773	776	782	rBV2	191	253	0.03%	0.003%
15	4.026	846	851	857	rVB2	312	370	0.04%	0.005%
16	4.152	887	890	892	rBV	271	200	0.02%	0.003%
17	4.531	1003	1008	1012	rVB2	211	223	0.02%	0.003%
18	4.563	1012	1018	1022	rBV2	176	265	0.03%	0.004%
19	4.612	1023	1033	1057	rBV	56750	149075	15.59%	2.016%
20	5.052	1155	1170	1195	rBV	164841	373561	39.07%	5.052%
21	5.280	1239	1241	1246	rVB3	347	190	0.02%	0.003%
22	5.473	1295	1301	1303	rBV2	243	240	0.03%	0.003%
23	5.534	1314	1320	1326	rBV	282	409	0.04%	0.006%
24	5.718	1356	1377	1405	rBV2	347753	956032	100.00%	12.928%
25	5.994	1460	1463	1465	rBV3	362	250	0.03%	0.003%
26	6.123	1501	1503	1506	rVB	314	214	0.02%	0.003%
27	6.177	1518	1520	1526	rVB2	279	227	0.02%	0.003%
28	6.242	1526	1540	1567	rBV	348007	678030	70.92%	9.169%
29	6.534	1623	1631	1639	rVB7	1975	3740	0.39%	0.051%
30	6.570	1639	1642	1648	rBV2	252	298	0.03%	0.004%
31	6.682	1664	1677	1708	rBV	215627	435632	45.57%	5.891%
32	6.849	1727	1729	1734	rVB3	486	288	0.03%	0.004%
33	6.927	1750	1753	1758	rVB2	190	191	0.02%	0.003%
34	6.959	1758	1763	1765	rBV2	297	261	0.03%	0.004%
35	7.197	1831	1837	1843	rVB3	405	573	0.06%	0.008%
36	7.271	1856	1860	1863	rBV	336	311	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
 Data File : VU057920.D
 Acq On : 22 Feb 2024 10:51
 Operator : MD/SY
 Sample : VU0222WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK043

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

37	7.309	1870	1872	1879	rBV2	156	195	0.02%	0.003%
38	7.367	1885	1890	1893	rBV2	219	235	0.02%	0.003%
39	7.560	1938	1950	1978	rBV	119362	222013	23.22%	3.002%
40	7.785	2016	2020	2021	rBV	476	291	0.03%	0.004%
41	7.891	2041	2053	2082	rBV	419940	750805	78.53%	10.153%
42	8.174	2130	2141	2162	rBV	77288	142685	14.92%	1.929%
43	8.383	2201	2206	2210	rBV2	244	283	0.03%	0.004%
44	8.521	2246	2249	2254	rVB2	261	227	0.02%	0.003%
45	8.550	2254	2258	2264	rBV2	1066	996	0.10%	0.013%
46	8.627	2271	2282	2324	rBV3	171461	389934	40.79%	5.273%
47	8.914	2368	2371	2374	rBV2	322	277	0.03%	0.004%
48	8.965	2380	2387	2390	rVB2	212	243	0.03%	0.003%
49	8.984	2390	2393	2397	rBV2	207	223	0.02%	0.003%
50	9.074	2417	2421	2425	rBV2	296	313	0.03%	0.004%
51	9.177	2448	2453	2457	rBV2	230	235	0.02%	0.003%
52	9.232	2467	2470	2475	rVV	167	173	0.02%	0.002%
53	9.299	2488	2491	2494	rVB	277	176	0.02%	0.002%
54	9.325	2494	2499	2502	rBV2	214	216	0.02%	0.003%
55	9.412	2512	2526	2567	rVV	477385	826632	86.46%	11.178%
56	9.570	2570	2575	2584	rVV3	1361	1736	0.18%	0.023%
57	9.695	2606	2614	2616	rBV3	1014	1081	0.11%	0.015%
58	9.759	2630	2634	2639	rBV2	263	281	0.03%	0.004%
59	9.904	2675	2679	2681	rBV	251	175	0.02%	0.002%
60	10.010	2705	2712	2715	rBV2	321	379	0.04%	0.005%
61	10.097	2734	2739	2742	rBV3	729	815	0.09%	0.011%
62	10.209	2772	2774	2777	rBV	210	170	0.02%	0.002%
63	10.373	2823	2825	2833	rVB	189	193	0.02%	0.003%
64	10.483	2852	2859	2860	rBV2	726	606	0.06%	0.008%
65	10.515	2866	2869	2872	rBV2	200	178	0.02%	0.002%
66	10.573	2883	2887	2890	rBV2	313	332	0.03%	0.004%
67	10.637	2902	2907	2915	rBV4	1281	1987	0.21%	0.027%
68	10.750	2930	2942	2963	rBV	250297	415497	43.46%	5.619%
69	10.852	2971	2974	2978	rVB2	275	239	0.02%	0.003%
70	11.039	3028	3032	3037	rVB2	217	233	0.02%	0.003%
71	11.373	3133	3136	3140	rBV	194	215	0.02%	0.003%
72	11.470	3160	3166	3176	rVB	1509	2328	0.24%	0.031%
73	11.531	3181	3185	3189	rBV2	210	254	0.03%	0.003%
74	11.579	3195	3200	3205	rVB2	249	297	0.03%	0.004%
75	11.672	3225	3229	3232	rBV2	221	189	0.02%	0.003%
76	11.746	3237	3252	3259	rBV4	2802	4433	0.46%	0.060%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
 Data File : VU057920.D
 Acq On : 22 Feb 2024 10:51
 Operator : MD/SY
 Sample : VU0222WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK043

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

77	11.807	3259	3271	3295	rBV	458565	764552	79.97%	10.339%
78	12.058	3346	3349	3351	rBV	217	178	0.02%	0.002%
79	12.187	3376	3389	3410	rBV	363578	614587	64.29%	8.311%
80	12.479	3477	3480	3482	rBV2	233	190	0.02%	0.003%
81	12.508	3486	3489	3495	rBV	184	177	0.02%	0.002%
82	12.631	3523	3527	3531	rBV2	251	303	0.03%	0.004%
83	12.656	3532	3535	3539	rVB2	241	228	0.02%	0.003%
84	13.052	3655	3658	3663	rVB2	211	248	0.03%	0.003%
85	13.077	3663	3666	3669	rBV	201	187	0.02%	0.003%
86	13.229	3704	3713	3722	rVB5	2825	4639	0.49%	0.063%
87	13.405	3763	3768	3770	rBV	311	294	0.03%	0.004%
88	13.653	3841	3845	3849	rBV2	284	331	0.03%	0.004%
89	13.695	3855	3858	3859	rBV	287	188	0.02%	0.003%
90	13.720	3862	3866	3868	rBV2	244	245	0.03%	0.003%
91	13.846	3896	3905	3914	rBV3	6976	10469	1.10%	0.142%
92	13.926	3927	3930	3936	rVB2	251	230	0.02%	0.003%
93	14.003	3951	3954	3956	rBV	263	176	0.02%	0.002%
94	14.093	3975	3982	3991	rBV2	7421	13180	1.38%	0.178%
95	14.184	4007	4010	4017	rVB3	345	238	0.02%	0.003%
96	14.328	4046	4055	4067	rVB6	6831	11798	1.23%	0.160%
97	14.431	4084	4087	4089	rBV	275	171	0.02%	0.002%
98	14.582	4132	4134	4138	rBV2	278	217	0.02%	0.003%
99	15.698	4478	4481	4484	rBV3	507	387	0.04%	0.005%
100	16.232	4645	4647	4650	rBV2	595	307	0.03%	0.004%




Sum of corrected areas: 7394930

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
Data File : VU057920.D
Acq On : 22 Feb 2024 10:51
Operator : MD/SY
Sample : VU0222WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK043

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

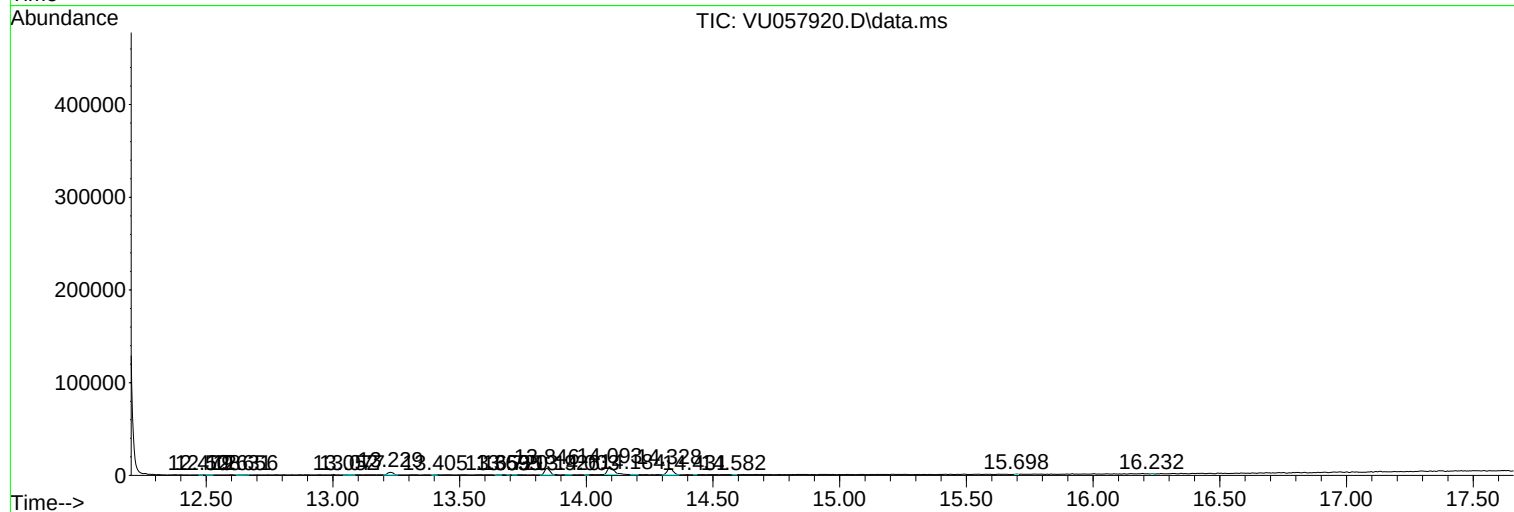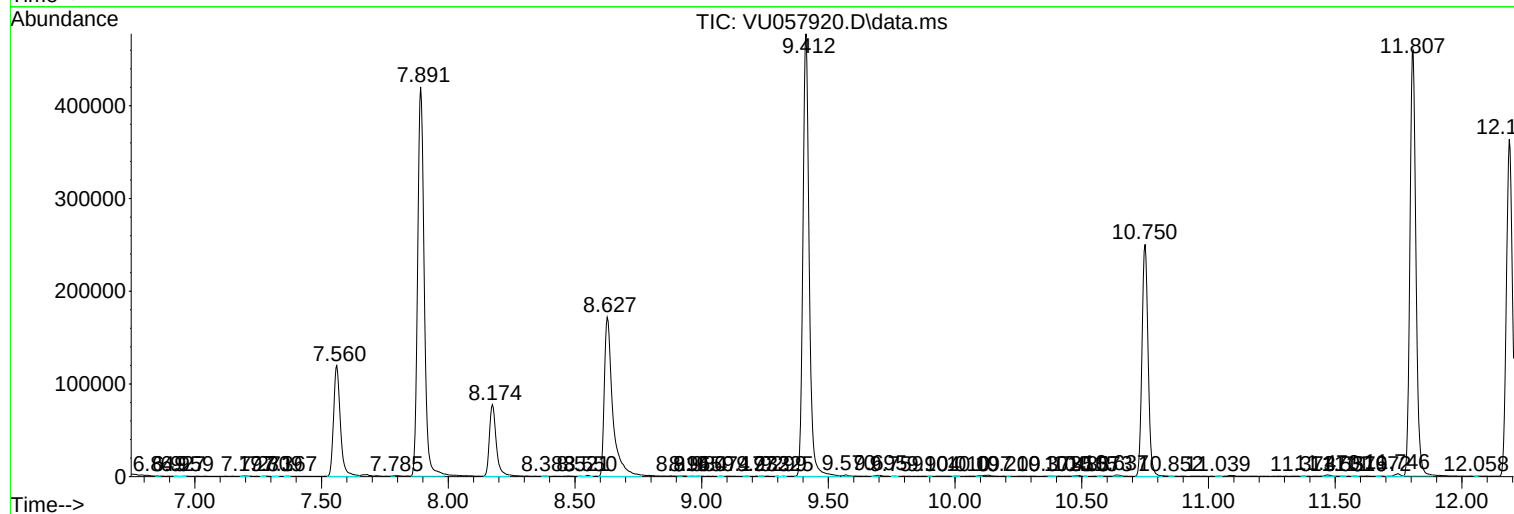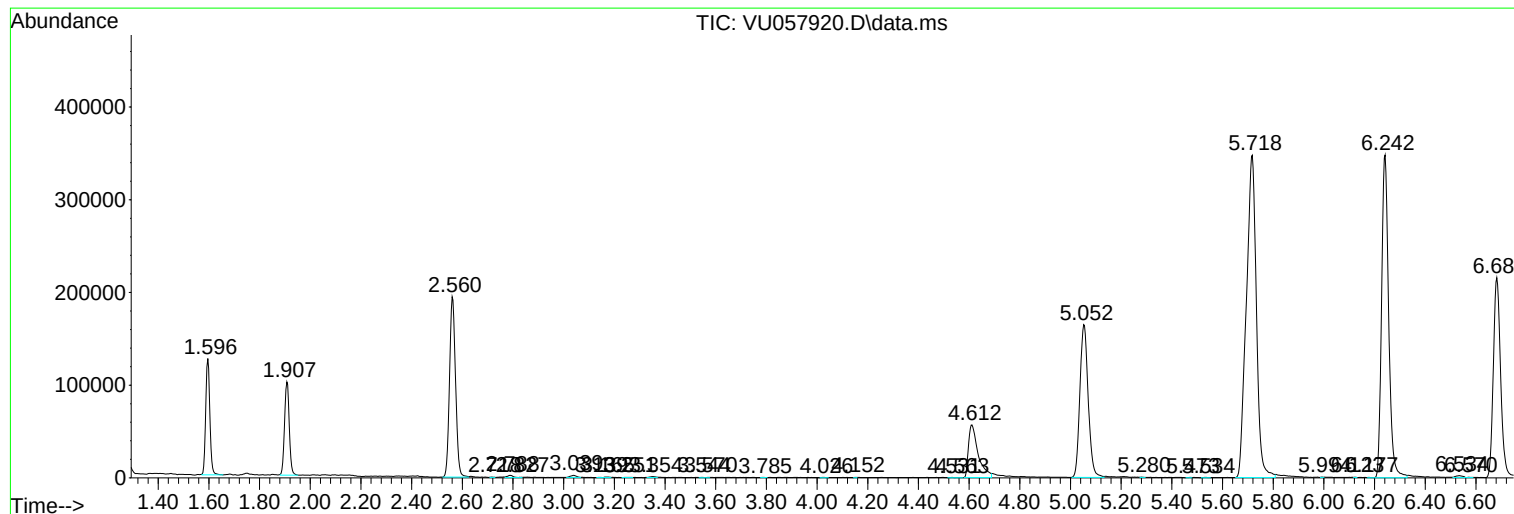

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
Data File : VU057920.D
Acq On : 22 Feb 2024 10:51
Operator : MD/SY
Sample : VU0222WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK043

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
Data File : VU057920.D
Acq On : 22 Feb 2024 10:51
Operator : MD/SY
Sample : VU0222WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK043

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------