

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
 Data File : VU057923.D
 Acq On : 22 Feb 2024 14:33
 Operator : MD/SY
 Sample : P1567-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JWAD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

Signal : TIC: VU057923.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	113	rVB	116173	133603	14.60%	1.837%
2	1.679	117	121	130	rVB	4030	4050	0.44%	0.056%
3	1.907	184	192	208	rVB	92977	120280	13.14%	1.654%
4	2.560	382	395	407	rBV	180227	299470	32.73%	4.118%
5	2.737	442	450	460	rBV	5944	11175	1.22%	0.154%
6	2.914	502	505	510	rVB2	320	295	0.03%	0.004%
7	3.039	536	544	553	rVB3	1636	2700	0.30%	0.037%
8	3.174	574	586	602	rVB4	1541	4319	0.47%	0.059%
9	3.351	638	641	645	rVB3	310	214	0.02%	0.003%
10	3.380	647	650	652	rBV	276	217	0.02%	0.003%
11	3.451	668	672	675	rBV2	220	244	0.03%	0.003%
12	3.534	693	698	700	rBV	244	240	0.03%	0.003%
13	3.856	795	798	805	rVB2	208	214	0.02%	0.003%
14	3.940	820	824	827	rBV2	240	219	0.02%	0.003%
15	4.013	844	847	849	rBV	259	184	0.02%	0.003%
16	4.055	857	860	864	rBV2	276	263	0.03%	0.004%
17	4.161	887	893	897	rBV2	214	310	0.03%	0.004%
18	4.419	966	973	974	rBV	1282	1275	0.14%	0.018%
19	4.493	994	996	1002	rVB	257	177	0.02%	0.002%
20	4.612	1019	1033	1061	rBV	60897	161023	17.60%	2.214%
21	4.843	1102	1105	1109	rBV3	647	549	0.06%	0.008%
22	5.052	1154	1170	1192	rBV	159995	360273	39.37%	4.954%
23	5.718	1356	1377	1413	rBV2	329723	915074	100.00%	12.583%
24	6.165	1512	1516	1521	rBV3	264	254	0.03%	0.003%
25	6.242	1527	1540	1569	rBV	351608	682521	74.59%	9.385%
26	6.531	1622	1630	1639	rBV4	1107	1708	0.19%	0.023%
27	6.634	1658	1662	1664	rBV2	337	227	0.02%	0.003%
28	6.682	1664	1677	1697	rBV	206883	412815	45.11%	5.676%
29	6.840	1724	1726	1731	rVB	469	341	0.04%	0.005%
30	6.862	1731	1733	1735	rBV2	261	176	0.02%	0.002%
31	6.878	1735	1738	1739	rVV2	406	238	0.03%	0.003%
32	6.901	1742	1745	1749	rVV3	369	363	0.04%	0.005%
33	7.126	1801	1815	1820	rBV7	2093	3812	0.42%	0.052%
34	7.190	1830	1835	1836	rBV4	324	186	0.02%	0.003%
35	7.415	1901	1905	1910	rVB2	253	253	0.03%	0.003%
36	7.441	1910	1913	1919	rBV	209	269	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
 Data File : VU057923.D
 Acq On : 22 Feb 2024 14:33
 Operator : MD/SY
 Sample : P1567-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JWAD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

37	7.502	1926	1932	1937	rVB2	201	226	0.02%	0.003%
38	7.560	1937	1950	1980	rBV	114871	212095	23.18%	2.916%
39	7.676	1980	1986	1991	rVV2	1642	1735	0.19%	0.024%
40	7.791	2017	2022	2027	rBV2	459	541	0.06%	0.007%
41	7.891	2041	2053	2088	rBV	405907	722663	78.97%	9.937%
42	8.174	2130	2141	2163	rBV2	76240	137287	15.00%	1.888%
43	8.373	2200	2203	2206	rBV	277	224	0.02%	0.003%
44	8.460	2223	2230	2232	rBV3	232	266	0.03%	0.004%
45	8.560	2257	2261	2270	rVB2	392	448	0.05%	0.006%
46	8.627	2270	2282	2322	rBV3	180453	409968	44.80%	5.637%
47	8.788	2327	2332	2347	rVB4	2526	4610	0.50%	0.063%
48	8.952	2381	2383	2386	rVV	269	175	0.02%	0.002%
49	9.010	2394	2401	2405	rVB2	274	369	0.04%	0.005%
50	9.045	2405	2412	2417	rBV2	296	550	0.06%	0.008%
51	9.142	2432	2442	2447	rBV2	363	647	0.07%	0.009%
52	9.338	2498	2503	2505	rBV	266	198	0.02%	0.003%
53	9.412	2513	2526	2566	rVV	479380	834004	91.14%	11.468%
54	9.605	2584	2586	2593	rVB3	408	294	0.03%	0.004%
55	9.663	2600	2604	2608	rBV	237	208	0.02%	0.003%
56	9.692	2608	2613	2614	rBV	506	399	0.04%	0.005%
57	9.824	2650	2654	2657	rBV	208	210	0.02%	0.003%
58	9.904	2673	2679	2685	rVB2	267	398	0.04%	0.005%
59	10.042	2719	2722	2726	rVB2	306	254	0.03%	0.003%
60	10.097	2735	2739	2741	rBV3	329	289	0.03%	0.004%
61	10.161	2756	2759	2763	rBV2	209	208	0.02%	0.003%
62	10.296	2796	2801	2804	rBV2	186	182	0.02%	0.003%
63	10.367	2820	2823	2830	rVB3	450	396	0.04%	0.005%
64	10.486	2854	2860	2864	rBV	389	430	0.05%	0.006%
65	10.541	2874	2877	2882	rBV2	284	349	0.04%	0.005%
66	10.666	2913	2916	2918	rBV	313	207	0.02%	0.003%
67	10.750	2929	2942	2965	rVV	250390	409831	44.79%	5.635%
68	10.881	2977	2983	2985	rBV2	465	433	0.05%	0.006%
69	10.984	3011	3015	3020	rBV2	232	203	0.02%	0.003%
70	11.087	3044	3047	3049	rBV	282	218	0.02%	0.003%
71	11.196	3075	3081	3085	rVB2	301	300	0.03%	0.004%
72	11.315	3115	3118	3119	rBV2	361	192	0.02%	0.003%
73	11.489	3161	3172	3191	rBV4	1958	4352	0.48%	0.060%
74	11.743	3245	3251	3259	rVB4	1054	1215	0.13%	0.017%
75	11.807	3259	3271	3298	rBV	485022	788507	86.17%	10.842%
76	11.981	3319	3325	3330	rBV3	255	364	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
 Data File : VU057923.D
 Acq On : 22 Feb 2024 14:33
 Operator : MD/SY
 Sample : P1567-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JWAD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

77	12.187	3377	3389	3415	rBV	362555	607182	66.35%	8.349%
78	12.396	3450	3454	3459	rVB2	424	427	0.05%	0.006%
79	12.422	3459	3462	3466	rBV2	255	278	0.03%	0.004%
80	12.499	3484	3486	3489	rVB2	356	211	0.02%	0.003%
81	12.524	3489	3494	3497	rBV2	346	402	0.04%	0.006%
82	12.762	3566	3568	3573	rVB3	329	266	0.03%	0.004%
83	12.794	3573	3578	3580	rBV2	258	234	0.03%	0.003%
84	12.875	3599	3603	3606	rBV	249	230	0.03%	0.003%
85	13.132	3677	3683	3686	rBV2	365	353	0.04%	0.005%
86	13.222	3707	3711	3712	rBV2	381	261	0.03%	0.004%
87	13.290	3728	3732	3735	rBV2	222	230	0.03%	0.003%
88	13.679	3850	3853	3857	rBV	212	176	0.02%	0.002%
89	13.856	3901	3908	3915	rBV6	1245	1831	0.20%	0.025%
90	13.975	3943	3945	3951	rVB	345	289	0.03%	0.004%
91	14.029	3959	3962	3964	rBV2	257	177	0.02%	0.002%
92	14.065	3970	3973	3975	rBV	396	238	0.03%	0.003%
93	14.335	4050	4057	4066	rVB4	1549	2050	0.22%	0.028%
94	14.396	4071	4076	4079	rBV3	413	405	0.04%	0.006%
95	14.476	4094	4101	4105	rBV3	412	660	0.07%	0.009%
96	14.566	4126	4129	4132	rVB2	334	207	0.02%	0.003%
97	15.479	4410	4413	4415	rBV	392	301	0.03%	0.004%
98	15.714	4483	4486	4491	rBV3	454	391	0.04%	0.005%
99	16.045	4586	4589	4593	rBV4	699	501	0.05%	0.007%
100	16.199	4634	4637	4639	rBV2	494	295	0.03%	0.004%




Sum of corrected areas: 7272571

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
Data File : VU057923.D
Acq On : 22 Feb 2024 14:33
Operator : MD/SY
Sample : P1567-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JWAD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

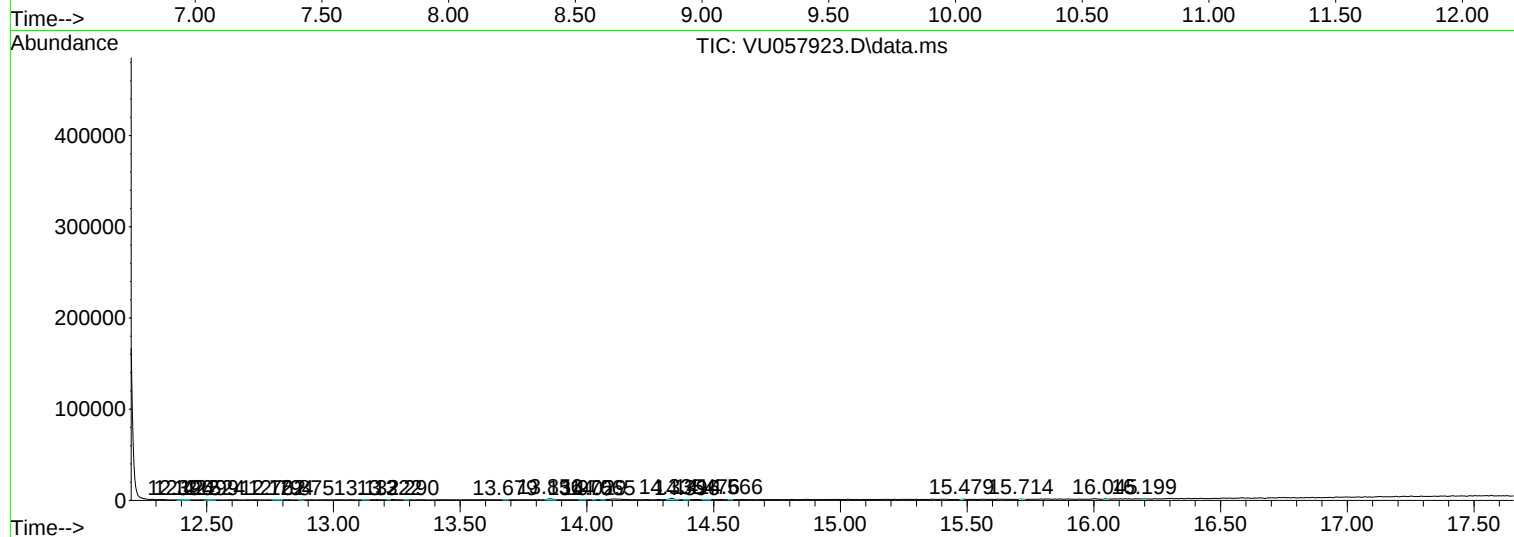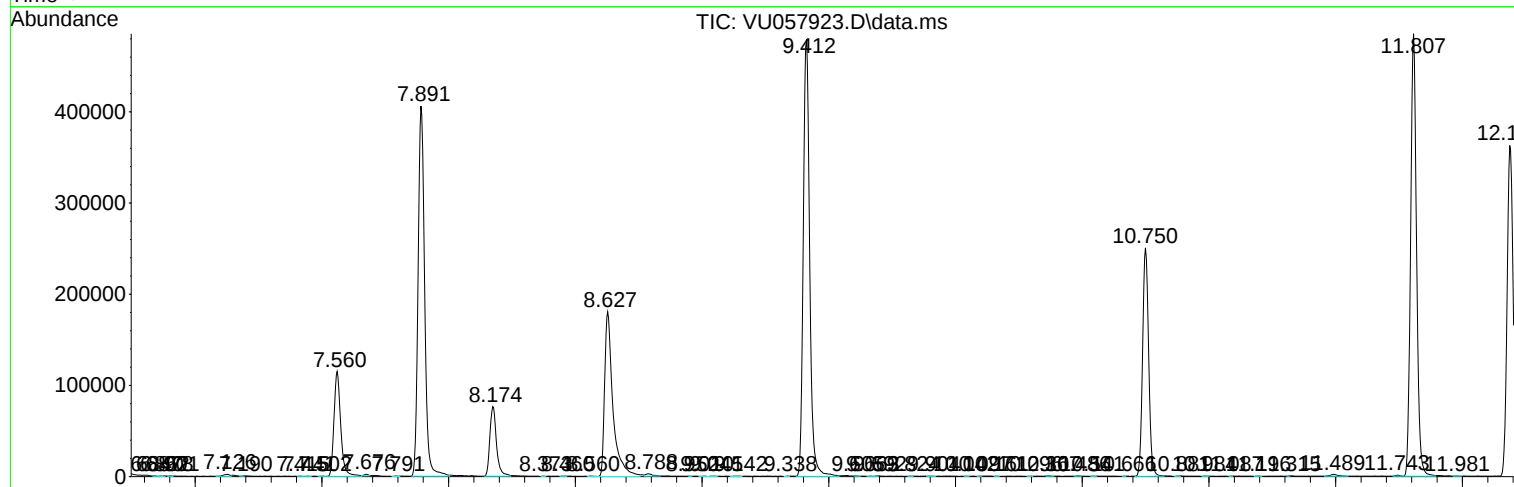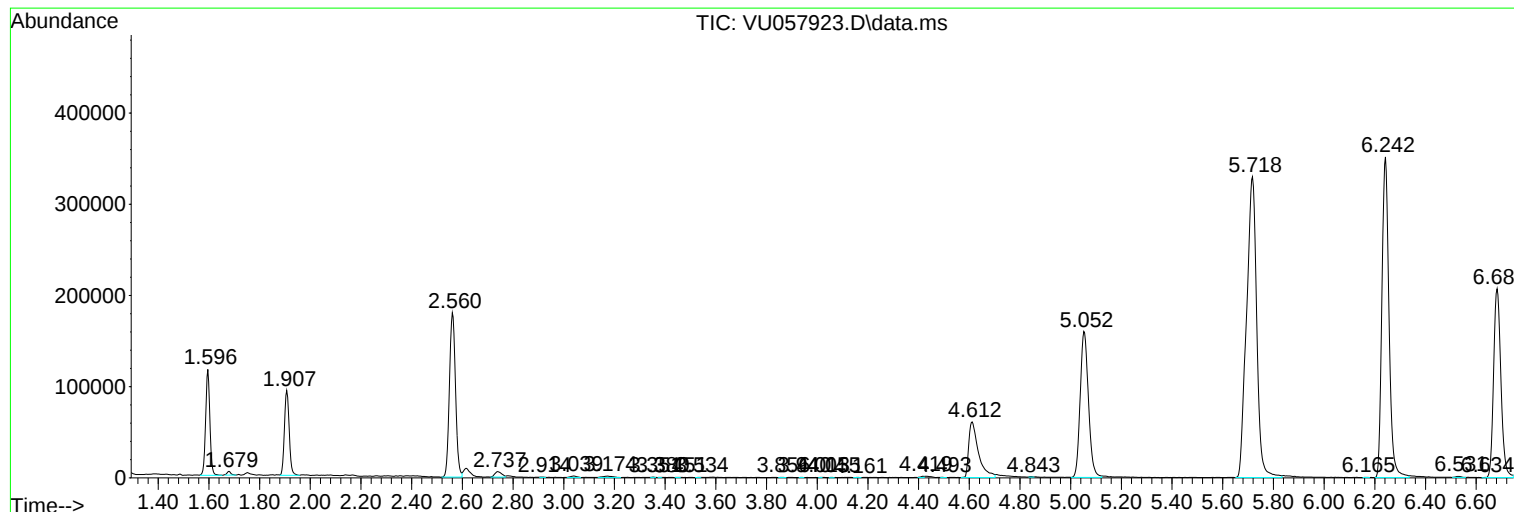

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
Data File : VU057923.D
Acq On : 22 Feb 2024 14:33
Operator : MD/SY
Sample : P1567-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JWAD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
Data File : VU057923.D
Acq On : 22 Feb 2024 14:33
Operator : MD/SY
Sample : P1567-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JWAD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------