

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
 Data File : VU057925.D
 Acq On : 22 Feb 2024 15:21
 Operator : MD/SY
 Sample : P1567-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JWAB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

Signal : TIC: VU057925.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	111	rVB	115437	132034	14.30%	1.817%
2	1.908	184	192	213	rVB	94431	121431	13.15%	1.671%
3	2.499	374	376	379	rVB	450	206	0.02%	0.003%
4	2.560	382	395	408	rBV	185673	303529	32.87%	4.177%
5	2.737	441	450	462	rBV	11484	22595	2.45%	0.311%
6	3.036	536	543	551	rVV3	1984	3237	0.35%	0.045%
7	3.171	574	585	599	rVB2	1551	3457	0.37%	0.048%
8	3.451	670	672	676	rBV2	194	175	0.02%	0.002%
9	3.522	692	694	697	rBV2	198	141	0.02%	0.002%
10	3.563	704	707	711	rBV	182	140	0.02%	0.002%
11	3.592	713	716	721	rVB2	305	245	0.03%	0.003%
12	4.078	861	867	869	rBV	256	295	0.03%	0.004%
13	4.612	1022	1033	1062	rBV	59702	159330	17.25%	2.193%
14	5.052	1155	1170	1198	rBV	161639	364648	39.49%	5.018%
15	5.345	1257	1261	1265	rVB2	214	141	0.02%	0.002%
16	5.370	1265	1269	1270	rBV2	227	144	0.02%	0.002%
17	5.412	1277	1282	1284	rBV2	379	337	0.04%	0.005%
18	5.428	1284	1287	1292	rVV2	170	179	0.02%	0.002%
19	5.502	1305	1310	1314	rVB	250	295	0.03%	0.004%
20	5.525	1314	1317	1320	rBV	283	254	0.03%	0.003%
21	5.557	1325	1327	1330	rBV	209	144	0.02%	0.002%
22	5.718	1356	1377	1415	rBV2	334135	923494	100.00%	12.709%
23	5.927	1440	1442	1444	rBV2	312	173	0.02%	0.002%
24	6.039	1472	1477	1479	rBV2	225	182	0.02%	0.003%
25	6.123	1499	1503	1507	rVB2	291	288	0.03%	0.004%
26	6.242	1526	1540	1565	rBV	347949	674927	73.08%	9.289%
27	6.489	1615	1617	1621	rBV3	227	181	0.02%	0.002%
28	6.521	1624	1627	1630	rBV4	467	367	0.04%	0.005%
29	6.589	1643	1648	1652	rVB2	128	154	0.02%	0.002%
30	6.682	1661	1677	1710	rBV	212730	420805	45.57%	5.791%
31	6.978	1766	1769	1772	rBV	193	178	0.02%	0.002%
32	7.148	1820	1822	1823	rBV	399	194	0.02%	0.003%
33	7.158	1823	1825	1828	rVB2	443	290	0.03%	0.004%
34	7.200	1834	1838	1840	rBV3	343	241	0.03%	0.003%
35	7.235	1846	1849	1852	rVB2	290	156	0.02%	0.002%
36	7.338	1877	1881	1887	rBV2	207	214	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
 Data File : VU057925.D
 Acq On : 22 Feb 2024 15:21
 Operator : MD/SY
 Sample : P1567-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JWAB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

37	7.364	1887	1889	1896	rBV2	112	155	0.02%	0.002%
38	7.441	1908	1913	1917	rVB2	176	195	0.02%	0.003%
39	7.560	1937	1950	1978	rBV	115096	211969	22.95%	2.917%
40	7.788	2018	2021	2024	rBV	252	151	0.02%	0.002%
41	7.808	2024	2027	2029	rBV3	254	162	0.02%	0.002%
42	7.891	2040	2053	2075	rBV	410556	718113	77.76%	9.883%
43	8.126	2124	2126	2131	rVB2	291	182	0.02%	0.003%
44	8.174	2131	2141	2176	rBV2	75947	140179	15.18%	1.929%
45	8.319	2182	2186	2188	rBV2	270	182	0.02%	0.003%
46	8.399	2206	2211	2214	rBV	311	310	0.03%	0.004%
47	8.470	2225	2233	2239	rBV2	727	859	0.09%	0.012%
48	8.505	2239	2244	2247	rBV2	175	159	0.02%	0.002%
49	8.547	2250	2257	2267	rBV3	6789	11015	1.19%	0.152%
50	8.628	2271	2282	2318	rBV2	182319	403052	43.64%	5.547%
51	8.843	2347	2349	2352	rVB2	400	254	0.03%	0.003%
52	9.126	2433	2437	2440	rBV	274	287	0.03%	0.004%
53	9.222	2465	2467	2473	rBV2	182	188	0.02%	0.003%
54	9.412	2513	2526	2563	rBV	476482	827886	89.65%	11.394%
55	9.656	2600	2602	2605	rVB	254	155	0.02%	0.002%
56	9.682	2605	2610	2611	rBV2	344	322	0.03%	0.004%
57	9.701	2611	2616	2625	rVB4	518	709	0.08%	0.010%
58	9.926	2681	2686	2688	rBV	219	251	0.03%	0.003%
59	10.004	2702	2710	2717	rBV2	304	626	0.07%	0.009%
60	10.074	2726	2732	2734	rBV	218	222	0.02%	0.003%
61	10.107	2739	2742	2745	rVB2	202	170	0.02%	0.002%
62	10.126	2745	2748	2750	rBV2	418	313	0.03%	0.004%
63	10.261	2784	2790	2795	rBV	284	400	0.04%	0.006%
64	10.303	2799	2803	2808	rVB	238	245	0.03%	0.003%
65	10.348	2814	2817	2822	rBV2	203	220	0.02%	0.003%
66	10.483	2854	2859	2862	rBV2	291	269	0.03%	0.004%
67	10.750	2930	2942	2965	rVV	246016	412488	44.67%	5.677%
68	10.943	2999	3002	3005	rBV2	210	158	0.02%	0.002%
69	11.055	3032	3037	3040	rBV3	598	635	0.07%	0.009%
70	11.193	3076	3080	3085	rBV2	256	326	0.04%	0.004%
71	11.235	3090	3093	3099	rBV2	166	193	0.02%	0.003%
72	11.470	3163	3166	3169	rBV3	401	394	0.04%	0.005%
73	11.512	3177	3179	3184	rVB2	277	172	0.02%	0.002%
74	11.669	3225	3228	3231	rBV2	244	176	0.02%	0.002%
75	11.737	3246	3249	3252	rBV2	443	352	0.04%	0.005%
76	11.807	3258	3271	3293	rBV	476547	783175	84.81%	10.778%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
 Data File : VU057925.D
 Acq On : 22 Feb 2024 15:21
 Operator : MD/SY
 Sample : P1567-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JWAB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

77	11.984	3323	3326	3328	rVB2	316	140	0.02%	0.002%
78	12.081	3348	3356	3359	rBV3	1316	2012	0.22%	0.028%
79	12.187	3376	3389	3406	rBV	361854	604922	65.50%	8.325%
80	12.283	3417	3419	3424	rVB2	433	286	0.03%	0.004%
81	12.373	3445	3447	3450	rBV	315	214	0.02%	0.003%
82	12.393	3450	3453	3456	rVV2	213	164	0.02%	0.002%
83	12.508	3485	3489	3492	rBV2	303	233	0.03%	0.003%
84	12.676	3538	3541	3547	rVB	230	271	0.03%	0.004%
85	12.714	3547	3553	3558	rBV2	353	557	0.06%	0.008%
86	12.772	3564	3571	3583	rVB3	756	1343	0.15%	0.018%
87	13.026	3644	3650	3653	rBV2	291	393	0.04%	0.005%
88	13.409	3766	3769	3774	rVB2	174	138	0.01%	0.002%
89	13.852	3903	3907	3908	rBV2	673	441	0.05%	0.006%
90	13.965	3939	3942	3945	rBV2	351	215	0.02%	0.003%
91	13.981	3945	3947	3952	rVB2	264	181	0.02%	0.002%
92	14.058	3967	3971	3976	rVB2	463	529	0.06%	0.007%
93	14.200	4013	4015	4019	rVB	251	169	0.02%	0.002%
94	14.299	4044	4046	4050	rVB2	258	157	0.02%	0.002%
95	14.409	4077	4080	4084	rBV	362	279	0.03%	0.004%
96	14.450	4089	4093	4095	rBV2	260	207	0.02%	0.003%
97	14.566	4122	4129	4131	rBV3	485	659	0.07%	0.009%
98	14.608	4140	4142	4144	rBV	431	281	0.03%	0.004%
99	14.759	4186	4189	4192	rBV2	308	196	0.02%	0.003%
100	15.052	4278	4280	4282	rBV2	324	165	0.02%	0.002%




Sum of corrected areas: 7266222

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
Data File : VU057925.D
Acq On : 22 Feb 2024 15:21
Operator : MD/SY
Sample : P1567-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JWAB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

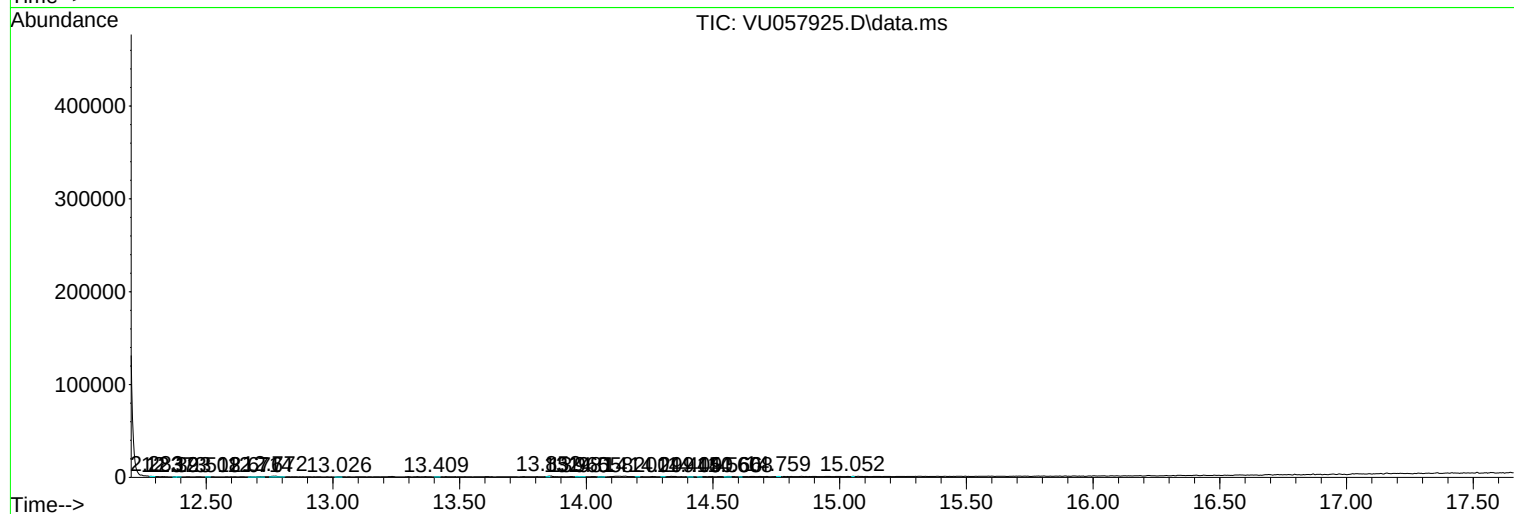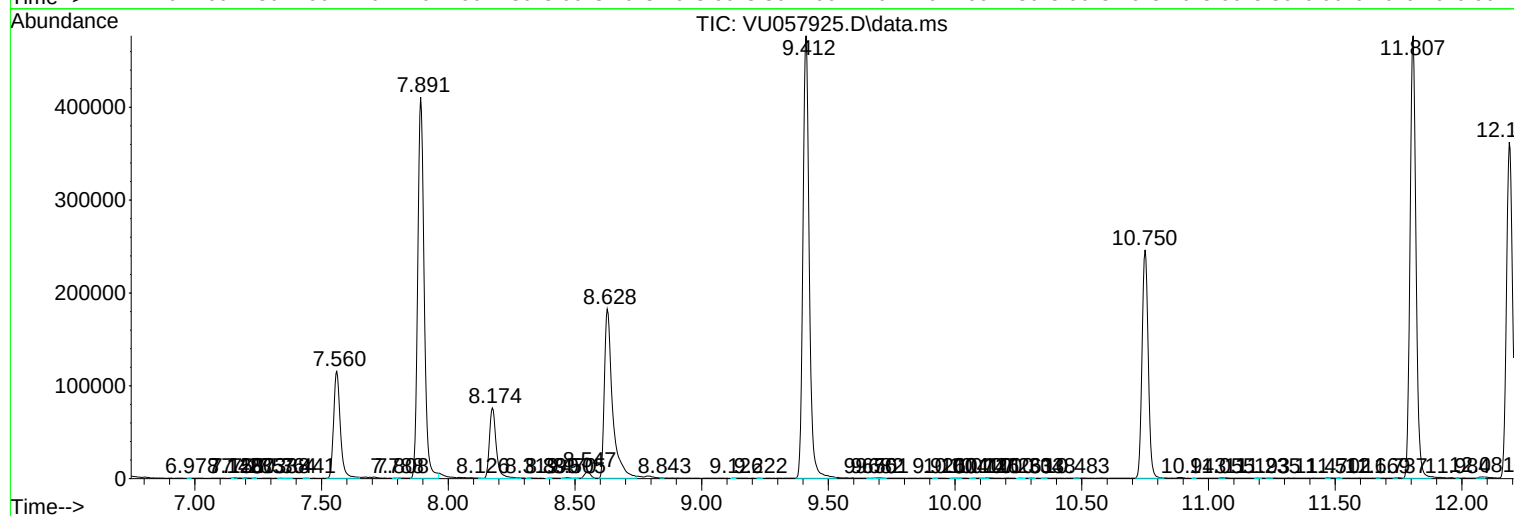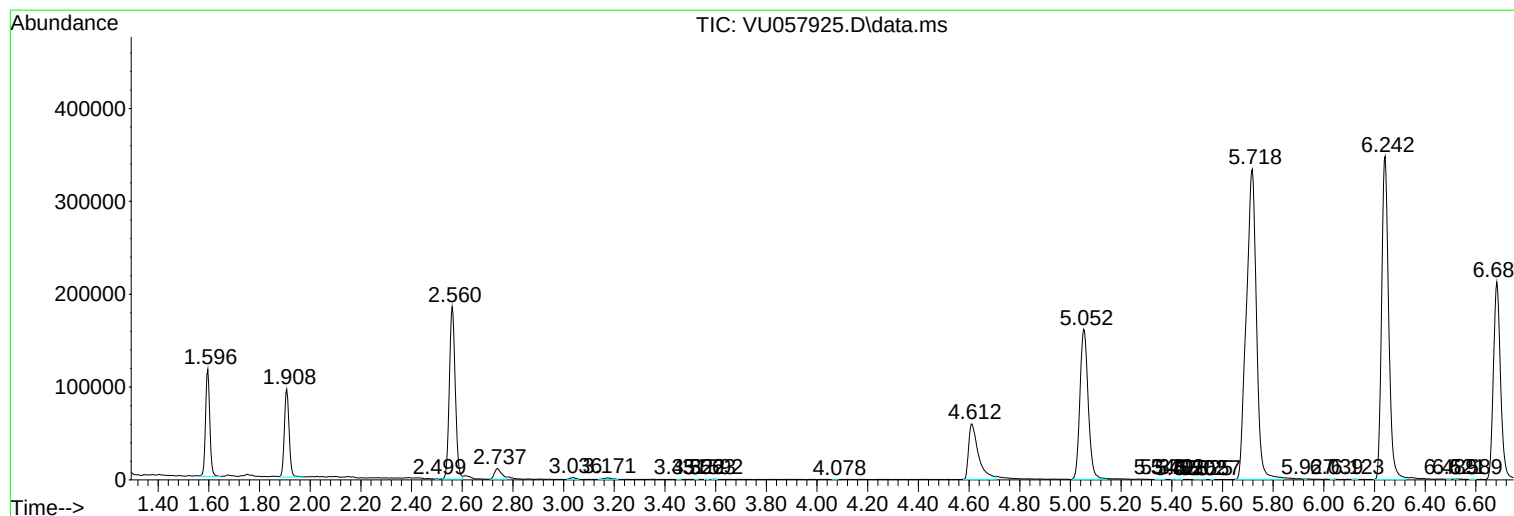

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
Data File : VU057925.D
Acq On : 22 Feb 2024 15:21
Operator : MD/SY
Sample : P1567-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JWAB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
Data File : VU057925.D
Acq On : 22 Feb 2024 15:21
Operator : MD/SY
Sample : P1567-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JWAB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc