

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
 Data File : VU057936.D
 Acq On : 22 Feb 2024 19:49
 Operator : MD/SY
 Sample : VIBLK043
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK043

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

Signal : TIC: VU057936.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	87	94	111	rVB	112108	127766	14.20%	1.800%
2	1.904	183	191	204	rVB	91777	118910	13.21%	1.675%
3	2.560	382	395	415	rBV	175365	292956	32.55%	4.128%
4	2.689	432	435	440	rVB3	343	286	0.03%	0.004%
5	2.744	445	452	460	rBV5	2350	3777	0.42%	0.053%
6	2.814	471	474	479	rBV3	261	225	0.03%	0.003%
7	2.985	525	527	530	rVV2	315	209	0.02%	0.003%
8	3.036	534	543	554	rVB4	3379	6039	0.67%	0.085%
9	3.168	578	584	585	rBV2	704	600	0.07%	0.008%
10	3.290	615	622	624	rBV	170	251	0.03%	0.004%
11	3.554	697	704	709	rBV2	353	607	0.07%	0.009%
12	3.644	728	732	736	rVB2	189	178	0.02%	0.003%
13	3.686	736	745	748	rBV2	266	393	0.04%	0.006%
14	3.824	785	788	794	rBV2	192	201	0.02%	0.003%
15	4.023	845	850	854	rBV2	232	301	0.03%	0.004%
16	4.049	854	858	862	rVV2	182	171	0.02%	0.002%
17	4.097	871	873	878	rVB2	273	222	0.02%	0.003%
18	4.171	892	896	898	rBV2	224	203	0.02%	0.003%
19	4.612	1019	1033	1066	rBV	59467	162734	18.08%	2.293%
20	5.052	1154	1170	1201	rBV	156223	353478	39.28%	4.980%
21	5.258	1232	1234	1239	rVB3	326	173	0.02%	0.002%
22	5.316	1247	1252	1258	rVB3	345	425	0.05%	0.006%
23	5.380	1269	1272	1277	rBV	214	199	0.02%	0.003%
24	5.502	1305	1310	1319	rBV	207	291	0.03%	0.004%
25	5.583	1329	1335	1338	rBV2	215	259	0.03%	0.004%
26	5.718	1356	1377	1417	rBV2	325677	899959	100.00%	12.680%
27	5.907	1434	1436	1439	rVB2	448	218	0.02%	0.003%
28	6.065	1480	1485	1489	rBV2	284	349	0.04%	0.005%
29	6.242	1525	1540	1568	rBV	346102	673975	74.89%	9.496%
30	6.470	1608	1611	1617	rVB3	451	333	0.04%	0.005%
31	6.525	1617	1628	1630	rBV6	1403	1593	0.18%	0.022%
32	6.621	1654	1658	1661	rBV2	201	185	0.02%	0.003%
33	6.682	1663	1677	1703	rBV	203926	404912	44.99%	5.705%
34	7.100	1800	1807	1812	rBV2	145	173	0.02%	0.002%
35	7.152	1820	1823	1829	rVV2	228	187	0.02%	0.003%
36	7.197	1833	1837	1841	rVV3	342	372	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
 Data File : VU057936.D
 Acq On : 22 Feb 2024 19:49
 Operator : MD/SY
 Sample : VIBLK043
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK043

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

37	7.329	1874	1878	1882	rVB2	182	190	0.02%	0.003%
38	7.351	1882	1885	1889	rBV2	228	222	0.02%	0.003%
39	7.419	1903	1906	1912	rVB2	259	236	0.03%	0.003%
40	7.489	1923	1928	1933	rBV2	231	305	0.03%	0.004%
41	7.560	1938	1950	1979	rBV	108146	202077	22.45%	2.847%
42	7.795	2020	2023	2031	rVB	308	245	0.03%	0.003%
43	7.891	2040	2053	2087	rBV	396953	702863	78.10%	9.903%
44	8.174	2130	2141	2166	rBV	74744	130342	14.48%	1.836%
45	8.300	2177	2180	2185	rVB3	350	359	0.04%	0.005%
46	8.467	2226	2232	2236	rBV2	299	401	0.04%	0.006%
47	8.544	2250	2256	2263	rBV	185	308	0.03%	0.004%
48	8.628	2271	2282	2317	rBV3	180315	400560	44.51%	5.644%
49	8.927	2373	2375	2379	rVB2	400	287	0.03%	0.004%
50	8.949	2379	2382	2385	rBV	227	191	0.02%	0.003%
51	9.187	2453	2456	2463	rVB2	315	399	0.04%	0.006%
52	9.219	2463	2466	2467	rBV	273	187	0.02%	0.003%
53	9.267	2477	2481	2484	rVB2	266	227	0.03%	0.003%
54	9.293	2484	2489	2493	rBV2	371	450	0.05%	0.006%
55	9.345	2499	2505	2508	rBV2	188	204	0.02%	0.003%
56	9.412	2513	2526	2550	rBV	477888	823616	91.52%	11.604%
57	9.563	2571	2573	2578	rVB2	303	204	0.02%	0.003%
58	9.695	2611	2614	2619	rBV3	304	268	0.03%	0.004%
59	9.775	2634	2639	2642	rBV2	395	408	0.05%	0.006%
60	9.869	2665	2668	2672	rBV	192	206	0.02%	0.003%
61	9.894	2672	2676	2682	rVB2	212	276	0.03%	0.004%
62	10.181	2759	2765	2768	rVB2	210	202	0.02%	0.003%
63	10.464	2848	2853	2857	rBV2	217	243	0.03%	0.003%
64	10.644	2903	2909	2913	rBV	251	256	0.03%	0.004%
65	10.750	2930	2942	2965	rBV	245882	405068	45.01%	5.707%
66	10.881	2979	2983	2984	rBV	308	218	0.02%	0.003%
67	10.962	3004	3008	3010	rBV	278	211	0.02%	0.003%
68	11.045	3031	3034	3039	rVB	204	176	0.02%	0.002%
69	11.139	3057	3063	3066	rBV2	222	214	0.02%	0.003%
70	11.418	3146	3150	3154	rVB2	295	219	0.02%	0.003%
71	11.557	3187	3193	3195	rBV2	189	235	0.03%	0.003%
72	11.743	3248	3251	3255	rBV2	556	423	0.05%	0.006%
73	11.808	3259	3271	3292	rBV	471588	772568	85.84%	10.885%
74	12.029	3333	3340	3344	rBV2	377	463	0.05%	0.007%
75	12.187	3377	3389	3417	rBV	349379	591073	65.68%	8.328%
76	12.634	3525	3528	3532	rVB2	270	187	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
 Data File : VU057936.D
 Acq On : 22 Feb 2024 19:49
 Operator : MD/SY
 Sample : VIBLK043
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK043

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

77	12.772	3566	3571	3575	rBV2	233	286	0.03%	0.004%
78	12.820	3584	3586	3592	rVB2	344	343	0.04%	0.005%
79	12.859	3593	3598	3602	rBV2	336	358	0.04%	0.005%
80	12.891	3602	3608	3611	rBV2	204	262	0.03%	0.004%
81	12.962	3627	3630	3636	rVB	206	213	0.02%	0.003%
82	13.589	3822	3825	3830	rBV	216	198	0.02%	0.003%
83	13.820	3895	3897	3903	rVV2	326	282	0.03%	0.004%
84	13.852	3905	3907	3910	rVV2	332	178	0.02%	0.003%
85	14.061	3969	3972	3976	rVB2	353	189	0.02%	0.003%
86	14.129	3990	3993	3996	rBV	313	201	0.02%	0.003%
87	14.325	4049	4054	4057	rBV2	518	598	0.07%	0.008%
88	14.467	4093	4098	4100	rBV	373	339	0.04%	0.005%
89	14.589	4133	4136	4139	rBV	424	358	0.04%	0.005%
90	14.640	4149	4152	4155	rBV2	324	205	0.02%	0.003%
91	14.669	4158	4161	4165	rBV	225	176	0.02%	0.002%
92	14.692	4165	4168	4171	rBV3	342	228	0.03%	0.003%
93	14.730	4176	4180	4183	rBV	223	233	0.03%	0.003%
94	14.836	4206	4213	4216	rBV3	451	582	0.06%	0.008%
95	15.319	4359	4363	4366	rBV2	452	421	0.05%	0.006%
96	15.470	4407	4410	4413	rBV2	342	273	0.03%	0.004%
97	15.611	4450	4454	4457	rBV	582	466	0.05%	0.007%
98	15.640	4460	4463	4466	rVV2	406	278	0.03%	0.004%
99	15.663	4466	4470	4472	rVB3	551	384	0.04%	0.005%
100	16.360	4684	4687	4689	rBV3	631	438	0.05%	0.006%




Sum of corrected areas: 7097386

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
Data File : VU057936.D
Acq On : 22 Feb 2024 19:49
Operator : MD/SY
Sample : VIBLK043
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK043

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

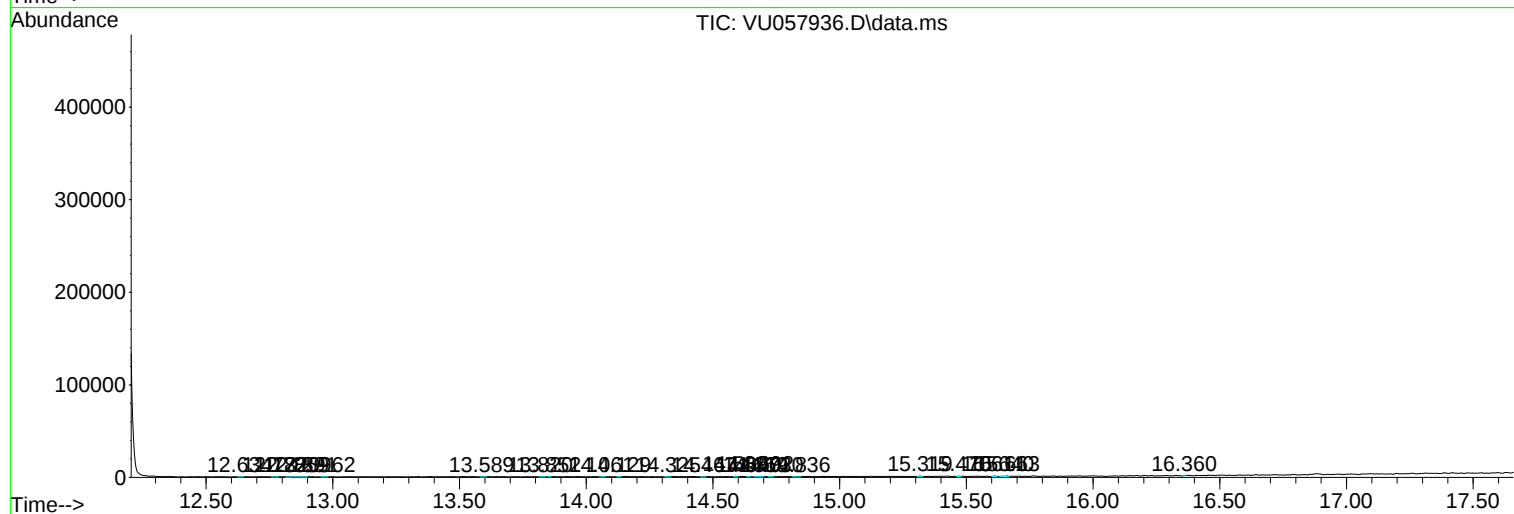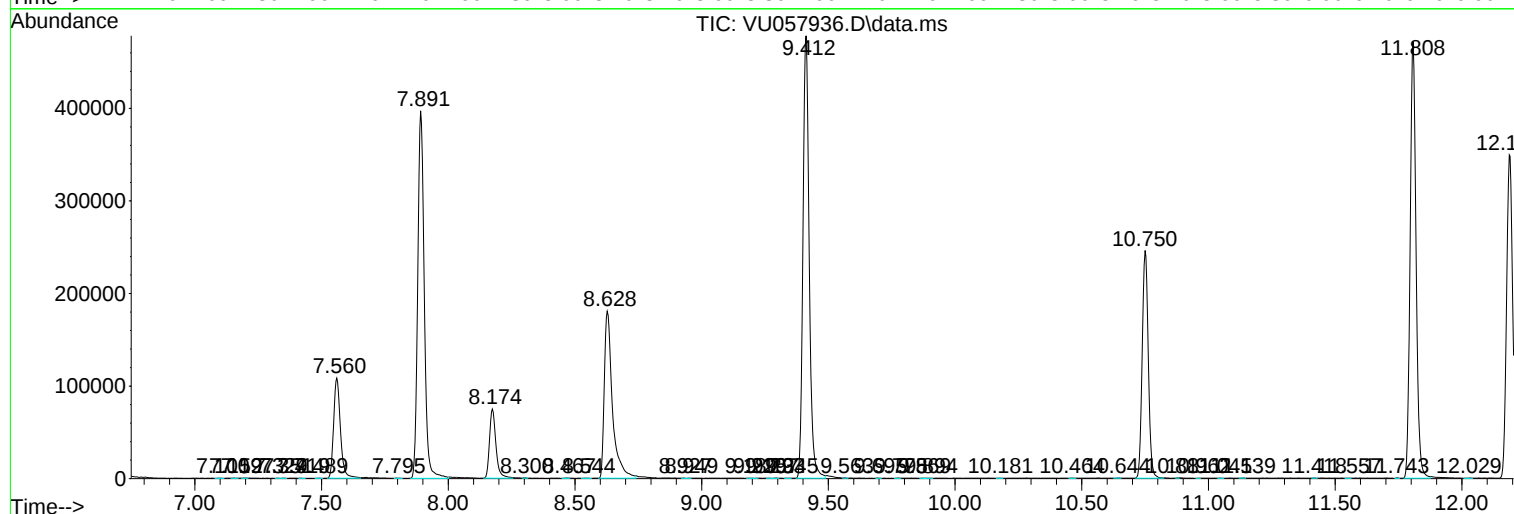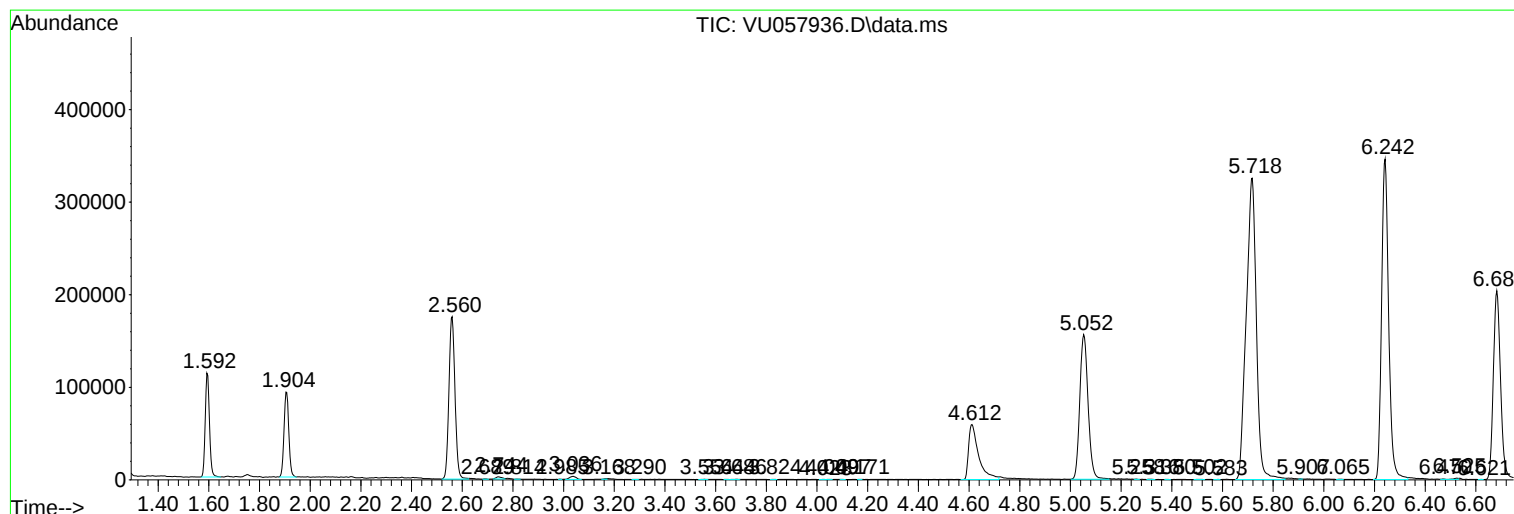

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
Data File : VU057936.D
Acq On : 22 Feb 2024 19:49
Operator : MD/SY
Sample : VIBLK043
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK043

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
Data File : VU057936.D
Acq On : 22 Feb 2024 19:49
Operator : MD/SY
Sample : VIBLK043
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK043

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------