
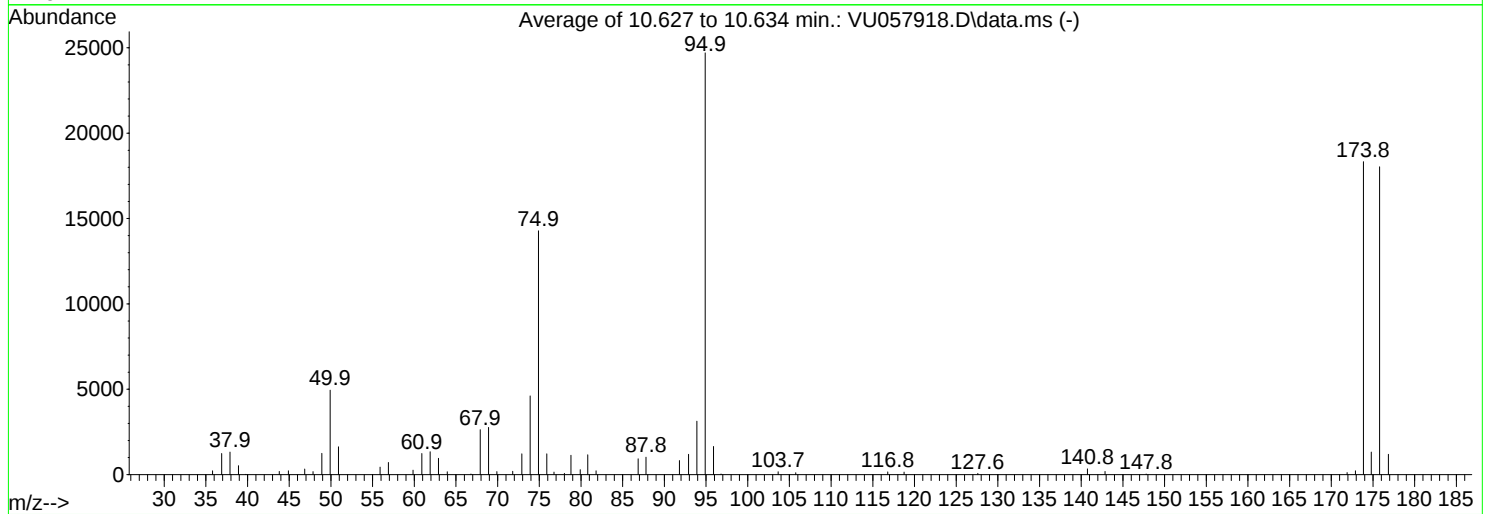


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022224\
Data File : VU057918.D
Acq On : 22 Feb 2024 08:36
Operator : MD/SY
Sample : BFB042
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB042

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Title : VOC Analysis
Last Update : Fri Feb 23 00:03:12 2024

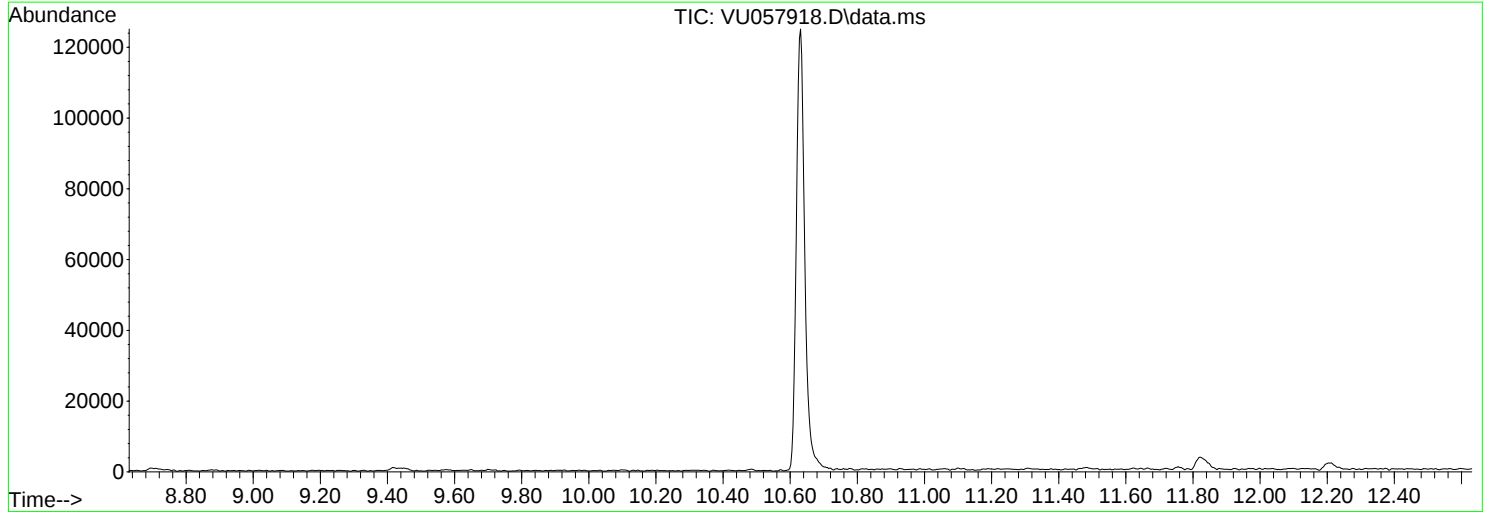

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2893

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	4946	PASS
75	95	30	80	57.8	14281	PASS
95	95	100	100	100.0	24704	PASS
96	95	5	9	6.7	1652	PASS
173	174	0.00	2	1.2	225	PASS
174	95	50	120	74.2	18331	PASS
175	174	5	9	7.2	1319	PASS
176	174	95	101	98.3	18027	PASS
177	176	5	9	6.6	1193	PASS

m/z	Abundance
35.80	121.0
39.90	113.0
43.90	306.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
35.90	324.0
36.90	1260.0
37.90	1366.0
38.90	533.0
39.80	108.0
43.80	492.0
44.90	255.0
46.90	335.0
47.90	175.0
48.90	1263.0
49.90	4986.0
50.90	1636.0
55.90	484.0
56.90	756.0
59.80	258.0
60.90	1259.0
61.90	1231.0
62.90	993.0
64.00	185.0
67.90	2683.0
68.90	2827.0
69.90	183.0
71.80	181.0
72.90	1185.0
73.90	4934.0
74.90	14401.0
75.90	1340.0
76.80	194.0
78.00	114.0
78.80	1131.0
79.90	233.0
80.80	1247.0
81.80	237.0
86.90	954.0
87.80	1046.0
91.80	781.0
92.90	1194.0
93.90	3211.0
94.90	25008.0
95.90	1661.0
103.70	145.0
105.80	117.0
116.80	168.0
118.90	146.0
140.80	384.0
142.90	171.0
147.80	101.0
171.90	112.0
172.90	233.0
173.90	18120.0
174.80	1357.0
175.80	17480.0
176.90	1230.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
35.90	377.0
36.90	1253.0
37.90	1339.0
38.90	548.0
39.70	142.0
43.80	503.0
44.90	232.0
46.80	309.0
47.80	178.0
48.90	1260.0
49.90	5076.0
50.90	1660.0
55.90	464.0
56.90	749.0
59.80	257.0
60.90	1263.0
61.90	1402.0
62.90	958.0
64.00	174.0
67.90	2717.0
68.90	2836.0
69.90	179.0
71.80	215.0
72.90	1268.0
73.90	4693.0
74.90	14675.0
75.90	1257.0
76.70	137.0
78.00	107.0
78.80	1165.0
79.90	293.0
80.80	1217.0
81.80	227.0
86.80	973.0
87.80	1064.0
91.80	871.0
92.90	1225.0
93.90	3208.0
94.90	25384.0
95.90	1733.0
103.60	172.0
105.80	115.0
116.80	161.0
118.70	147.0
127.60	101.0
140.70	351.0
142.80	186.0
171.90	135.0
172.90	233.0
173.90	18776.0
174.80	1349.0
175.80	18608.0
176.90	1222.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
35.80	346.0
36.90	1201.0
37.90	1252.0
38.90	485.0
39.70	154.0
43.80	492.0
44.90	199.0
46.80	327.0
47.80	177.0
48.90	1221.0
49.90	4776.0
50.90	1590.0
55.90	379.0
56.90	638.0
59.90	258.0
60.90	1189.0
61.90	1378.0
62.90	928.0
63.90	141.0
66.80	108.0
67.90	2486.0
68.90	2619.0
69.90	177.0
71.80	187.0
72.90	1208.0
73.90	4216.0
74.90	13767.0
75.90	1056.0
76.80	120.0
78.80	1106.0
79.90	352.0
80.80	1023.0
81.80	219.0
86.80	852.0
87.80	949.0
91.80	825.0
92.90	1159.0
93.90	2958.0
94.90	23720.0
95.90	1562.0
96.80	102.0
103.70	198.0
105.70	104.0
116.80	138.0
118.60	157.0
127.60	118.0
140.70	289.0
142.80	214.0
171.90	112.0
172.90	210.0
173.80	18096.0
174.80	1252.0
175.80	17992.0
176.80	1126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042