

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022321\
 Data File : VU042412.D
 Acq On : 23 Feb 2021 11:37
 Operator : SY/MD
 Sample : VU0223WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK111

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M

Title : VOC Analysis

Signal : TIC: VU042412.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	100	rVB	102887	122031	13.06%	1.699%
2	1.916	172	179	191	rVB	90049	116039	12.42%	1.616%
3	2.575	371	384	403	rBV	204746	346923	37.12%	4.831%
4	2.690	417	420	422	rBV	195	128	0.01%	0.002%
5	2.938	494	497	498	rBV	172	95	0.01%	0.001%
6	2.964	500	505	507	rBV2	250	240	0.03%	0.003%
7	3.195	569	577	582	rBV2	467	640	0.07%	0.009%
8	3.256	589	596	602	rBV2	246	297	0.03%	0.004%
9	3.382	630	635	638	rBV2	214	192	0.02%	0.003%
10	3.481	662	666	669	rBV	139	128	0.01%	0.002%
11	3.526	676	680	687	rBV2	167	145	0.02%	0.002%
12	3.616	705	708	711	rBV	155	120	0.01%	0.002%
13	3.655	717	720	723	rBV2	184	140	0.01%	0.002%
14	4.259	904	908	911	rBV2	273	212	0.02%	0.003%
15	4.279	912	914	918	rBV	111	98	0.01%	0.001%
16	4.340	931	933	937	rBV2	259	164	0.02%	0.002%
17	4.452	965	968	974	rVB2	232	228	0.02%	0.003%
18	4.536	992	994	998	rVB2	167	131	0.01%	0.002%
19	4.565	999	1003	1006	rBV2	150	138	0.01%	0.002%
20	4.636	1009	1025	1054	rBV2	94697	252748	27.05%	3.520%
21	4.951	1122	1123	1130	rVB	356	283	0.03%	0.004%
22	5.073	1144	1161	1183	rVV	171683	373676	39.99%	5.204%
23	5.176	1191	1193	1195	rBV	163	98	0.01%	0.001%
24	5.301	1221	1232	1239	rBV3	680	1360	0.15%	0.019%
25	5.385	1250	1258	1262	rBV3	688	1023	0.11%	0.014%
26	5.491	1288	1291	1294	rVB	179	113	0.01%	0.002%
27	5.568	1312	1315	1320	rBV2	147	94	0.01%	0.001%
28	5.597	1320	1324	1329	rBV2	187	149	0.02%	0.002%
29	5.735	1344	1367	1393	rBV2	338334	934486	100.00%	13.013%
30	5.954	1431	1435	1441	rBV3	282	330	0.04%	0.005%
31	6.054	1464	1466	1468	rBV2	402	204	0.02%	0.003%
32	6.083	1472	1475	1477	rBV2	177	139	0.01%	0.002%
33	6.124	1484	1488	1492	rBV3	374	272	0.03%	0.004%
34	6.144	1492	1494	1496	rBV2	257	170	0.02%	0.002%
35	6.182	1503	1506	1508	rBV2	248	139	0.01%	0.002%
36	6.256	1514	1529	1546	rBV	282371	538048	57.58%	7.493%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022321\
 Data File : VU042412.D
 Acq On : 23 Feb 2021 11:37
 Operator : SY/MD
 Sample : VU0223WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK111

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
 Title : VOC Analysis

37	6.539	1609	1617	1626	rVB3	2241	3702	0.40%	0.052%
38	6.700	1652	1667	1688	rVV	219612	426162	45.60%	5.934%
39	6.780	1690	1692	1695	rBV2	246	146	0.02%	0.002%
40	6.819	1700	1704	1710	rVB2	372	442	0.05%	0.006%
41	7.018	1763	1766	1770	rVV	200	129	0.01%	0.002%
42	7.054	1773	1777	1781	rBV	181	155	0.02%	0.002%
43	7.102	1789	1792	1795	rVB	218	121	0.01%	0.002%
44	7.124	1795	1799	1803	rBV	140	123	0.01%	0.002%
45	7.144	1803	1805	1808	rBV	222	130	0.01%	0.002%
46	7.179	1814	1816	1818	rBV	287	207	0.02%	0.003%
47	7.314	1856	1858	1862	rVB2	258	169	0.02%	0.002%
48	7.353	1862	1870	1872	rBV2	231	245	0.03%	0.003%
49	7.452	1899	1901	1905	rBV2	167	146	0.02%	0.002%
50	7.497	1912	1915	1921	rBV2	274	294	0.03%	0.004%
51	7.574	1926	1939	1962	rBV	128635	228735	24.48%	3.185%
52	7.729	1984	1987	1990	rVB2	301	176	0.02%	0.002%
53	7.803	2007	2010	2016	rVB3	405	352	0.04%	0.005%
54	7.906	2028	2042	2071	rBV	411161	722725	77.34%	10.064%
55	8.189	2118	2130	2151	rBV	90448	156650	16.76%	2.181%
56	8.353	2178	2181	2187	rVB2	191	119	0.01%	0.002%
57	8.385	2188	2191	2194	rBV	217	164	0.02%	0.002%
58	8.430	2202	2205	2209	rBV	114	110	0.01%	0.002%
59	8.475	2216	2219	2221	rBV	182	128	0.01%	0.002%
60	8.510	2226	2230	2231	rBV2	212	137	0.01%	0.002%
61	8.591	2251	2255	2258	rVB2	202	157	0.02%	0.002%
62	8.645	2258	2272	2301	rBV	304730	562525	60.20%	7.833%
63	8.867	2336	2341	2343	rBV2	249	211	0.02%	0.003%
64	8.970	2369	2373	2374	rBV	198	98	0.01%	0.001%
65	9.021	2385	2389	2393	rVB2	323	207	0.02%	0.003%
66	9.246	2455	2459	2464	rVB	268	212	0.02%	0.003%
67	9.308	2474	2478	2480	rBV2	175	159	0.02%	0.002%
68	9.423	2500	2514	2538	rBV	376091	640636	68.55%	8.921%
69	9.574	2556	2561	2567	rBV2	487	558	0.06%	0.008%
70	9.648	2579	2584	2588	rBV2	295	264	0.03%	0.004%
71	9.700	2594	2600	2607	rBV4	770	1117	0.12%	0.016%
72	9.996	2687	2692	2696	rBV2	200	232	0.02%	0.003%
73	10.031	2699	2703	2710	rBV2	285	349	0.04%	0.005%
74	10.115	2722	2729	2734	rBV2	513	592	0.06%	0.008%
75	10.172	2745	2747	2750	rVB	243	114	0.01%	0.002%
76	10.205	2755	2757	2760	rBV2	199	142	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022321\
 Data File : VU042412.D
 Acq On : 23 Feb 2021 11:37
 Operator : SY/MD
 Sample : VU0223WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK111

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
 Title : VOC Analysis

77	10.275	2776	2779	2782	rBV2	244	163	0.02%	0.002%
78	10.468	2837	2839	2842	rVV	225	107	0.01%	0.001%
79	10.568	2867	2870	2874	rBV2	198	186	0.02%	0.003%
80	10.639	2887	2892	2895	rVB2	437	316	0.03%	0.004%
81	10.719	2912	2917	2919	rBV2	274	222	0.02%	0.003%
82	10.764	2919	2931	2948	rVV	289937	466389	49.91%	6.495%
83	10.915	2975	2978	2985	rVB2	218	237	0.03%	0.003%
84	11.086	3027	3031	3033	rBV2	291	188	0.02%	0.003%
85	11.246	3078	3081	3083	rBV	195	122	0.01%	0.002%
86	11.381	3121	3123	3126	rVB	253	124	0.01%	0.002%
87	11.613	3193	3195	3199	rVB	224	105	0.01%	0.001%
88	11.745	3233	3236	3238	rBV2	433	324	0.03%	0.005%
89	11.819	3247	3259	3279	rBV	387803	617966	66.13%	8.605%
90	11.954	3297	3301	3304	rBV	271	215	0.02%	0.003%
91	12.201	3365	3378	3394	rBV	410216	650531	69.61%	9.059%
92	12.314	3410	3413	3417	rBV2	287	241	0.03%	0.003%
93	12.523	3475	3478	3485	rVB	325	323	0.03%	0.004%
94	13.095	3653	3656	3658	rBV	250	189	0.02%	0.003%
95	13.278	3711	3713	3716	rVB2	328	165	0.02%	0.002%
96	13.327	3725	3728	3731	rVB2	377	219	0.02%	0.003%
97	14.166	3986	3989	3995	rBV2	436	486	0.05%	0.007%
98	14.339	4040	4043	4049	rVB3	1528	1304	0.14%	0.018%
99	14.394	4058	4060	4062	rBV3	258	145	0.02%	0.002%
100	14.468	4080	4083	4087	rBV2	417	377	0.04%	0.005%


Sum of corrected areas: 7181105

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022321\
Data File : VU042412.D
Acq On : 23 Feb 2021 11:37
Operator : SY/MD
Sample : VU0223WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK111

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

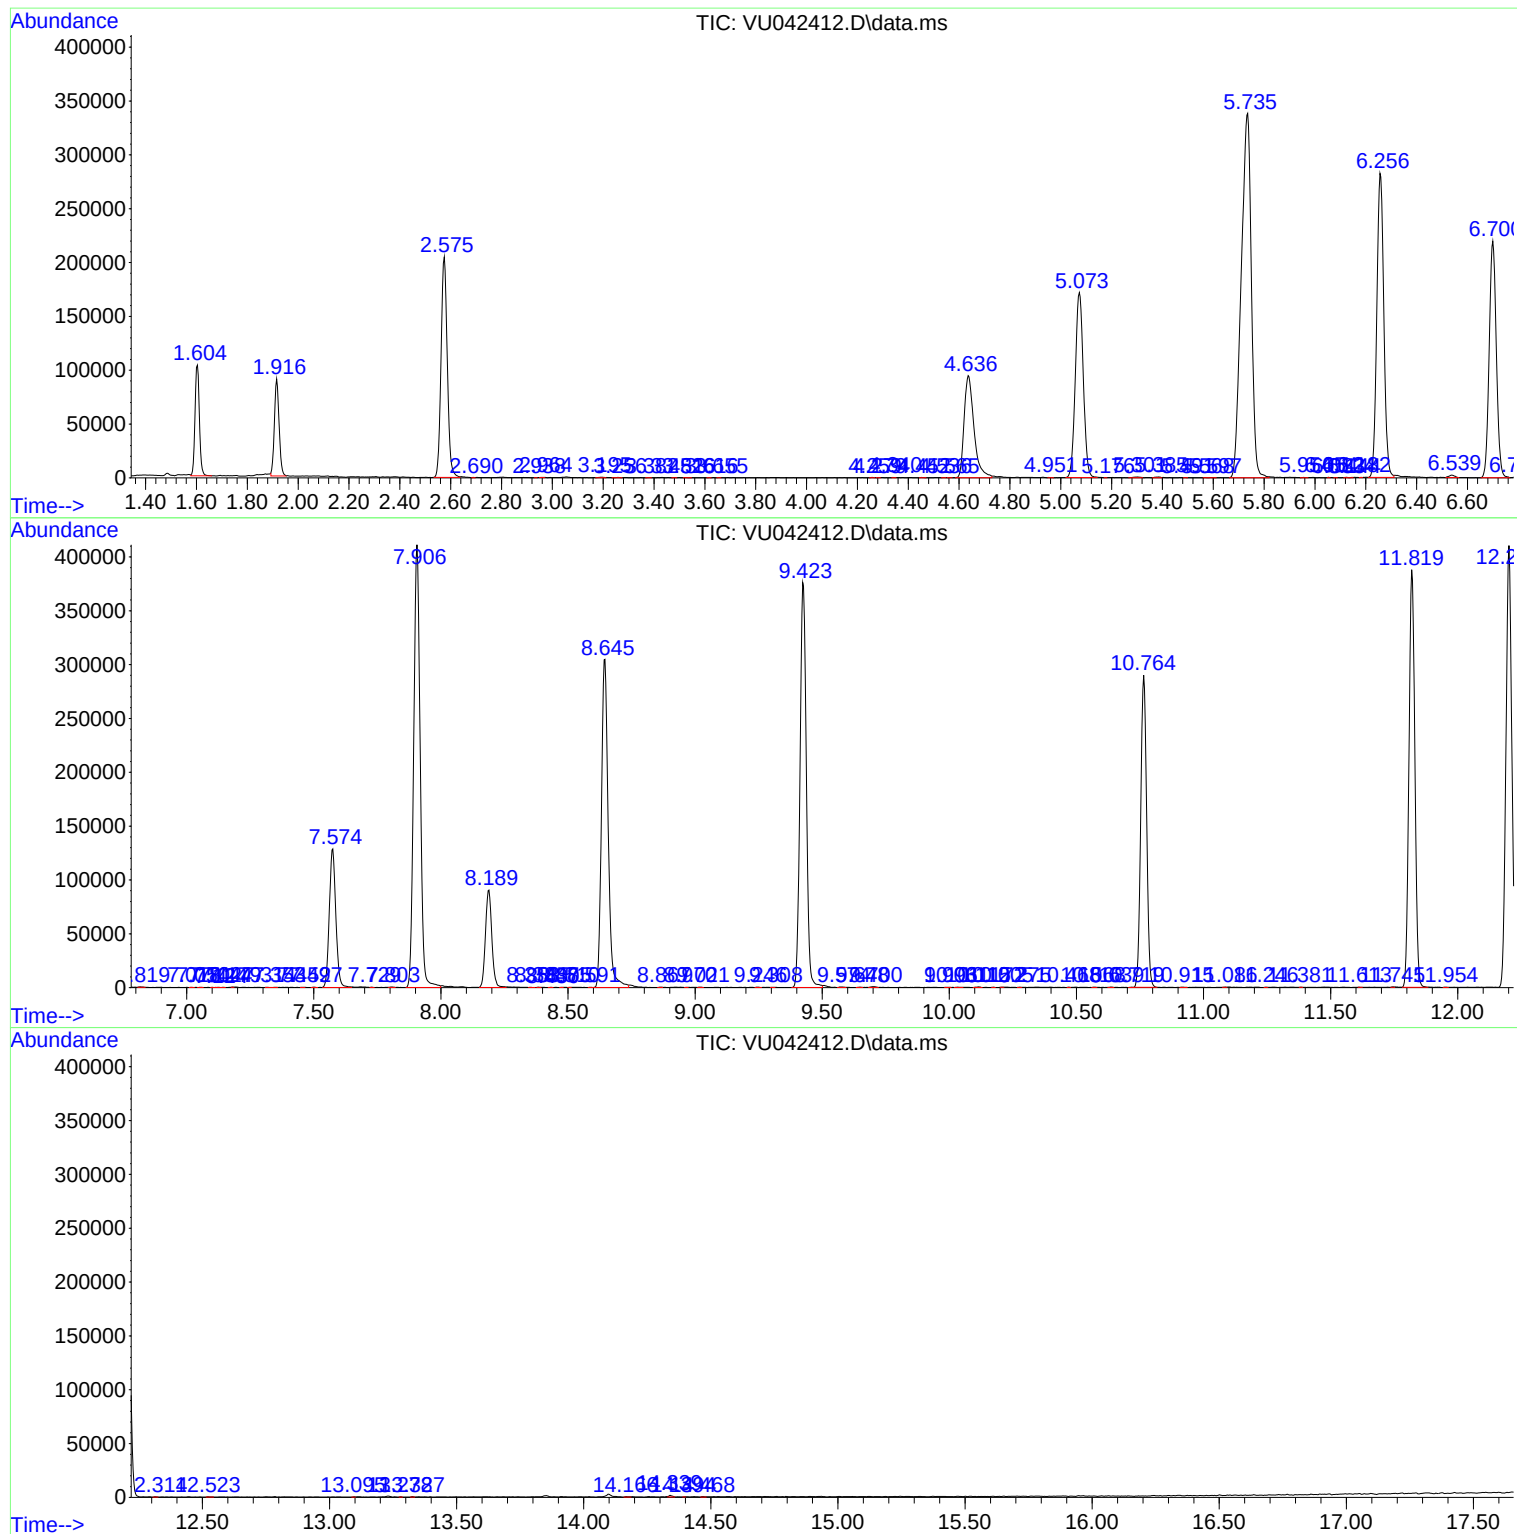

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022321\
Data File : VU042412.D
Acq On : 23 Feb 2021 11:37
Operator : SY/MD
Sample : VU0223WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK111

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022321\
Data File : VU042412.D
Acq On : 23 Feb 2021 11:37
Operator : SY/MD
Sample : VU0223WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK111

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
