

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022321\
 Data File : VU042413.D
 Acq On : 23 Feb 2021 12:00
 Operator : SY/MD
 Sample : VU0223MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
 Title : VOC Analysis

Signal : TIC: VU042413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	96	rVB	99500	116817	12.90%	1.675%
2	1.916	172	179	197	rVB	85104	114321	12.63%	1.640%
3	2.575	371	384	411	rBV	192845	334919	37.00%	4.804%
4	2.957	500	503	505	rBV2	327	243	0.03%	0.003%
5	3.044	526	530	531	rBV	561	347	0.04%	0.005%
6	3.202	570	579	585	rBV2	622	1164	0.13%	0.017%
7	3.469	660	662	664	rBV	169	110	0.01%	0.002%
8	3.604	701	704	707	rBV	225	128	0.01%	0.002%
9	3.616	707	708	713	rVB	141	82	0.01%	0.001%
10	3.684	726	729	733	rBV	442	427	0.05%	0.006%
11	3.764	751	754	756	rBV	163	87	0.01%	0.001%
12	3.932	804	806	810	rVB2	182	105	0.01%	0.002%
13	3.954	810	813	816	rBV2	172	177	0.02%	0.003%
14	4.141	867	871	873	rBV	191	173	0.02%	0.002%
15	4.182	882	884	890	rVB2	188	113	0.01%	0.002%
16	4.247	901	904	906	rBV2	150	92	0.01%	0.001%
17	4.288	913	917	920	rBV2	208	221	0.02%	0.003%
18	4.359	936	939	943	rBV2	177	170	0.02%	0.002%
19	4.440	963	964	965	rBV2	119	32	0.00%	0.000%
20	4.494	978	981	987	rVB2	312	249	0.03%	0.004%
21	4.523	987	990	993	rBV	179	89	0.01%	0.001%
22	4.639	1011	1026	1069	rBV	90642	257840	28.48%	3.698%
23	4.938	1115	1119	1121	rVB	192	143	0.02%	0.002%
24	4.954	1122	1124	1127	rBV2	201	104	0.01%	0.001%
25	4.993	1133	1136	1141	rVB2	200	159	0.02%	0.002%
26	5.073	1145	1161	1182	rBV	167403	362844	40.08%	5.204%
27	5.250	1214	1216	1218	rBV2	146	79	0.01%	0.001%
28	5.337	1242	1243	1245	rBV	109	25	0.00%	0.000%
29	5.472	1284	1285	1286	rBV	115	28	0.00%	0.000%
30	5.587	1318	1321	1322	rBV	154	112	0.01%	0.002%
31	5.655	1340	1342	1344	rBV	140	67	0.01%	0.001%
32	5.735	1344	1367	1390	rBV2	331603	905236	100.00%	12.984%
33	5.973	1439	1441	1443	rBV2	305	153	0.02%	0.002%
34	6.012	1450	1453	1456	rVB2	284	164	0.02%	0.002%
35	6.038	1456	1461	1462	rBV	427	278	0.03%	0.004%
36	6.073	1471	1472	1474	rBV	202	65	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022321\
 Data File : VU042413.D
 Acq On : 23 Feb 2021 12:00
 Operator : SY/MD
 Sample : VU0223MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK112

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
 Title : VOC Analysis

37	6.092	1475	1478	1481	rVB2	213	137	0.02%	0.002%
38	6.128	1486	1489	1493	rVB	529	416	0.05%	0.006%
39	6.150	1493	1496	1497	rBV	349	197	0.02%	0.003%
40	6.176	1501	1504	1508	rBV3	316	284	0.03%	0.004%
41	6.195	1508	1510	1511	rBV	329	127	0.01%	0.002%
42	6.256	1516	1529	1547	rBV	267647	499809	55.21%	7.169%
43	6.536	1608	1616	1624	rVB6	2320	3804	0.42%	0.055%
44	6.568	1624	1626	1627	rVB	115	44	0.00%	0.001%
45	6.700	1652	1667	1685	rBV	213327	414092	45.74%	5.939%
46	6.806	1696	1700	1701	rBV2	506	390	0.04%	0.006%
47	6.851	1712	1714	1717	rBV	225	154	0.02%	0.002%
48	6.902	1726	1730	1731	rBV	266	133	0.01%	0.002%
49	6.967	1748	1750	1754	rVB	234	94	0.01%	0.001%
50	7.031	1767	1770	1771	rBV	177	80	0.01%	0.001%
51	7.156	1807	1809	1810	rBV	147	44	0.00%	0.001%
52	7.189	1814	1819	1821	rVV2	434	479	0.05%	0.007%
53	7.214	1825	1827	1829	rBV	166	65	0.01%	0.001%
54	7.275	1843	1846	1848	rVB	186	79	0.01%	0.001%
55	7.362	1871	1873	1875	rVB	171	67	0.01%	0.001%
56	7.378	1875	1878	1881	rBV	197	113	0.01%	0.002%
57	7.439	1894	1897	1904	rVB2	220	173	0.02%	0.002%
58	7.497	1909	1915	1920	rBV	211	378	0.04%	0.005%
59	7.574	1925	1939	1964	rBV	124880	223560	24.70%	3.206%
60	7.764	1994	1998	2000	rBV	260	217	0.02%	0.003%
61	7.906	2029	2042	2067	rBV	396320	696932	76.99%	9.996%
62	8.185	2117	2129	2148	rBV	87434	152821	16.88%	2.192%
63	8.314	2167	2169	2171	rBV	329	177	0.02%	0.003%
64	8.356	2179	2182	2185	rBV	239	161	0.02%	0.002%
65	8.581	2251	2252	2253	rBV	117	31	0.00%	0.000%
66	8.645	2259	2272	2302	rBV	305624	559976	61.86%	8.032%
67	8.890	2345	2348	2352	rVB2	243	159	0.02%	0.002%
68	8.925	2352	2359	2362	rBV3	589	596	0.07%	0.009%
69	9.189	2438	2441	2442	rBV3	170	81	0.01%	0.001%
70	9.230	2448	2454	2458	rBV2	325	355	0.04%	0.005%
71	9.353	2490	2492	2497	rVB	228	112	0.01%	0.002%
72	9.427	2501	2515	2548	rBV	357925	614408	67.87%	8.812%
73	9.610	2569	2572	2575	rBV2	351	305	0.03%	0.004%
74	9.967	2680	2683	2691	rVB2	333	452	0.05%	0.006%
75	10.034	2702	2704	2708	rBV	214	131	0.01%	0.002%
76	10.124	2731	2732	2736	rBV2	379	232	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022321\
 Data File : VU042413.D
 Acq On : 23 Feb 2021 12:00
 Operator : SY/MD
 Sample : VU0223MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M

Title : VOC Analysis

77	10.484	2842	2844	2846	rBV	236	162	0.02%	0.002%
78	10.642	2890	2893	2898	rBV3	435	389	0.04%	0.006%
79	10.764	2918	2931	2951	rVB	288869	461984	51.03%	6.626%
80	11.304	3097	3099	3100	rBV	183	61	0.01%	0.001%
81	11.365	3115	3118	3122	rBV	277	178	0.02%	0.003%
82	11.385	3122	3124	3125	rBV	175	56	0.01%	0.001%
83	11.526	3166	3168	3173	rBV	166	93	0.01%	0.001%
84	11.819	3246	3259	3277	rVB	374132	591666	65.36%	8.486%
85	12.201	3365	3378	3393	rBV	408140	646397	71.41%	9.271%
86	12.751	3545	3549	3554	rBV2	345	385	0.04%	0.006%
87	13.851	3885	3891	3894	rBV2	851	911	0.10%	0.013%
88	14.053	3952	3954	3956	rBV	320	116	0.01%	0.002%
89	14.333	4039	4041	4045	rBV3	720	491	0.05%	0.007%




Sum of corrected areas: 6972117

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022321\
Data File : VU042413.D
Acq On : 23 Feb 2021 12:00
Operator : SY/MD
Sample : VU0223MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

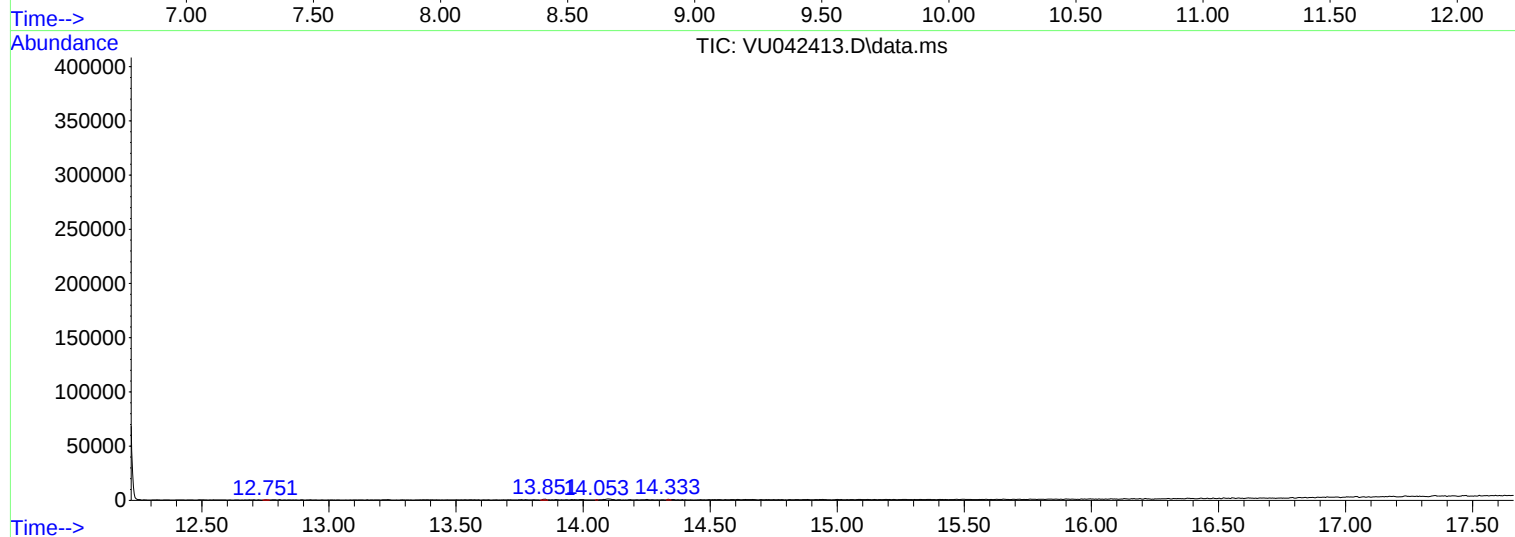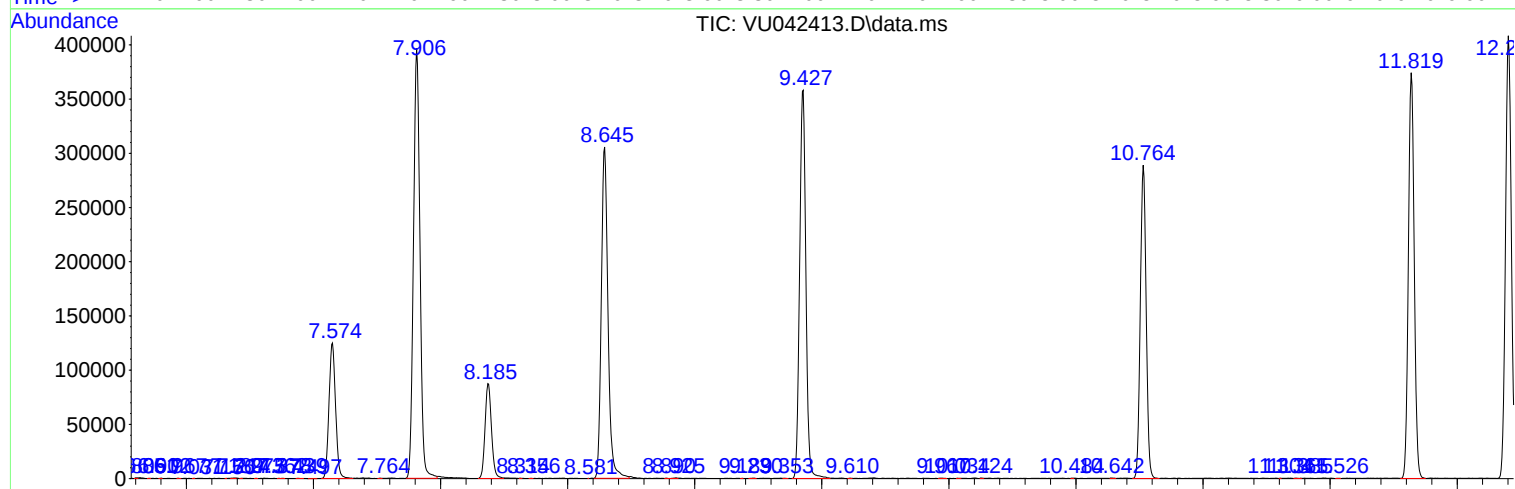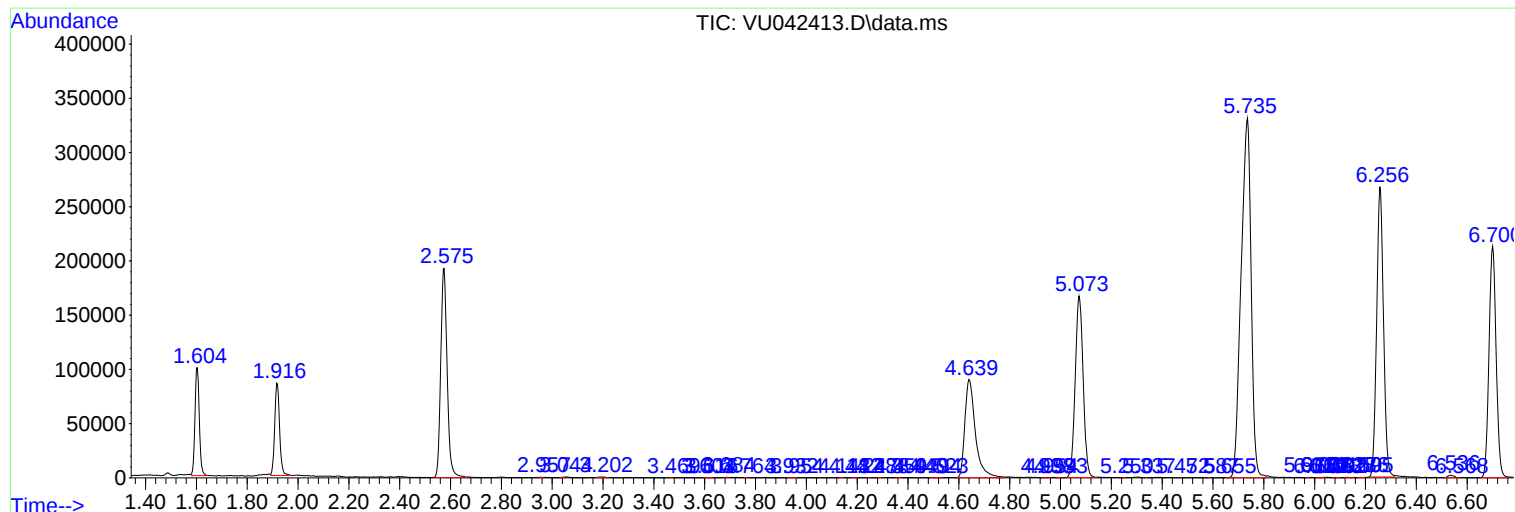

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022321\
Data File : VU042413.D
Acq On : 23 Feb 2021 12:00
Operator : SY/MD
Sample : VU0223MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022321\
Data File : VU042413.D
Acq On : 23 Feb 2021 12:00
Operator : SY/MD
Sample : VU0223MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
