
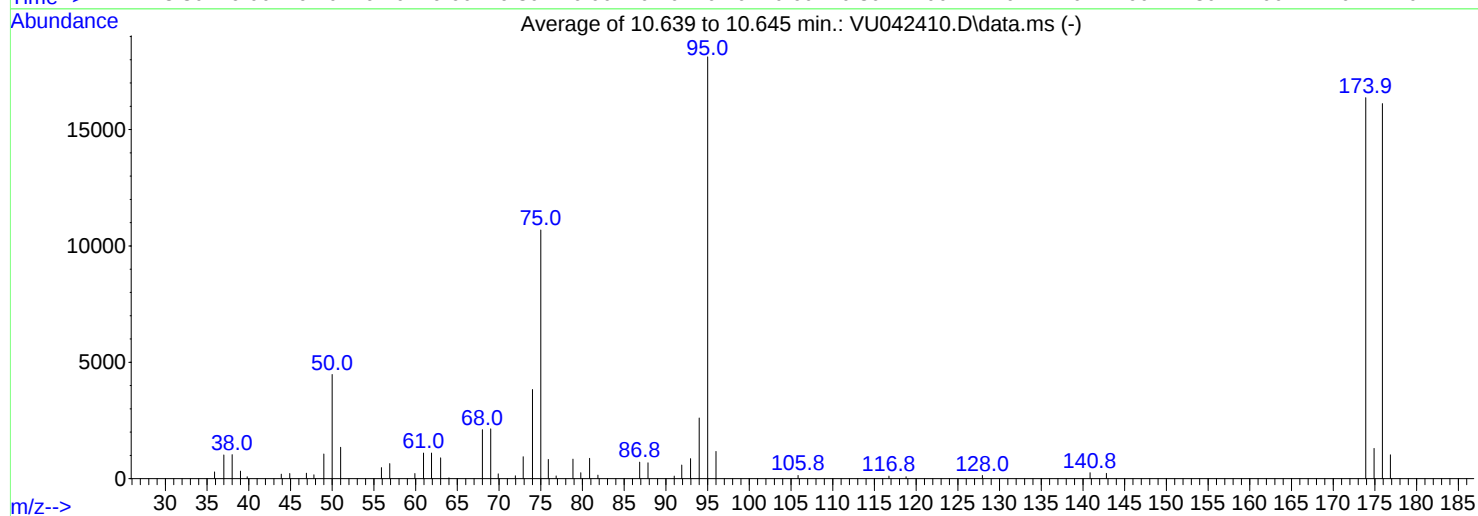


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022321\
 Data File : VU042410.D
 Acq On : 23 Feb 2021 10:13
 Operator : SY/MD
 Sample : BFB63
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB630

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
 Title : VOC Analysis
 Last Update : Wed Feb 24 03:51:21 2021

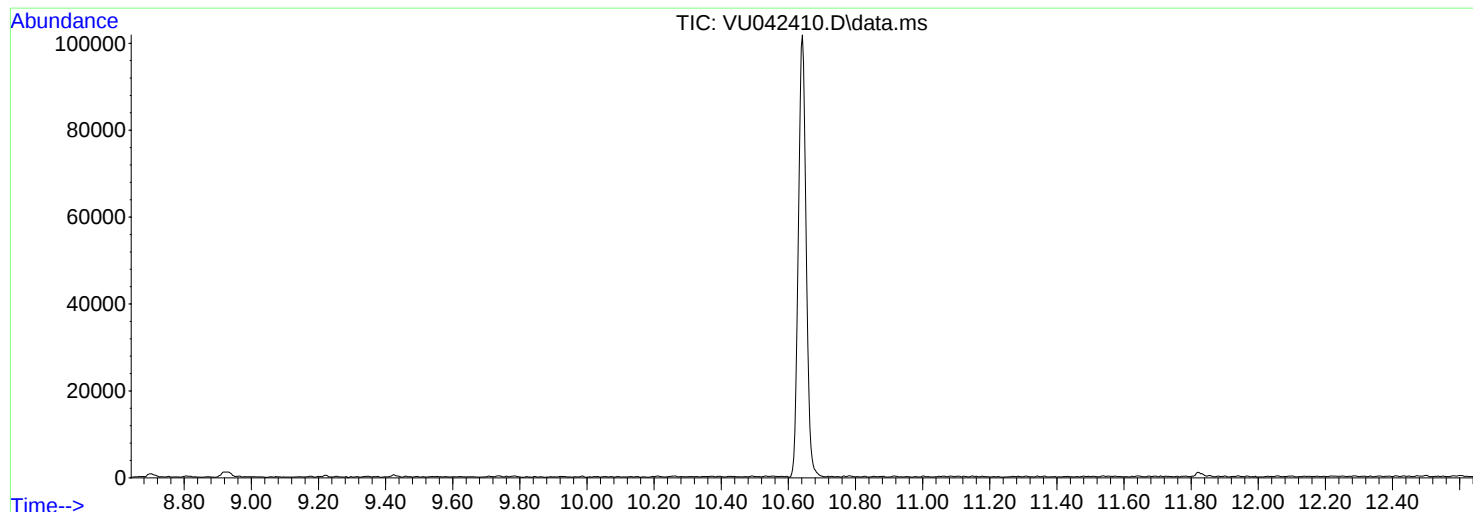

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.7	4477	PASS
75	95	30	80	58.9	10684	PASS
95	95	100	100	100.0	18125	PASS
96	95	5	9	6.4	1166	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.3	16373	PASS
175	174	5	9	7.9	1300	PASS
176	174	95	101	98.4	16115	PASS
177	176	5	9	6.3	1023	PASS

m/z	Abundance
35.90	361.0
37.00	1106.0
38.00	1065.0
39.00	323.0
43.90	375.0
44.90	216.0
46.90	292.0
47.80	171.0
49.00	1071.0
50.00	4454.0
51.00	1345.0
55.90	484.0
56.90	653.0
59.90	177.0
60.90	1125.0
61.90	1021.0
63.00	891.0
64.00	106.0
68.00	2151.0
69.00	2156.0
69.90	171.0
71.90	117.0
72.90	986.0
74.00	3730.0
75.00	10932.0
75.90	888.0
76.80	122.0
78.90	874.0
79.70	263.0
80.90	851.0
81.80	176.0
86.80	769.0
87.90	732.0
91.00	180.0
91.90	580.0
93.00	853.0
94.00	2655.0
95.00	18328.0
96.00	1243.0
105.90	143.0
116.80	121.0
127.90	147.0
140.90	241.0
142.80	215.0
173.90	15862.0
174.90	1400.0
175.90	16022.0
176.90	941.0

Instrument :
MSVOA_U
ClientSampleId :
BFB630

m/z	Abundance
35.90	307.0
37.00	1042.0
38.00	1057.0
39.00	317.0
39.80	115.0
43.90	363.0
44.90	237.0
46.90	237.0
47.80	175.0
49.00	1101.0
50.00	4699.0
51.00	1380.0
55.90	497.0
56.90	679.0
59.90	235.0
60.90	1113.0
61.90	1140.0
63.00	916.0
68.00	2185.0
69.00	2209.0
69.90	215.0
71.90	123.0
72.90	942.0
74.00	3997.0
75.00	11029.0
75.90	850.0
76.90	118.0
78.90	873.0
79.80	252.0
80.90	873.0
81.90	147.0
86.80	754.0
87.90	695.0
91.00	159.0
91.90	586.0
93.00	889.0
94.00	2703.0
95.00	18640.0
96.00	1216.0
105.90	150.0
116.70	111.0
118.80	115.0
127.90	152.0
140.80	243.0
142.80	243.0
173.90	16832.0
174.90	1334.0
175.90	16600.0
176.80	1024.0

Instrument :
MSVOA_U
ClientSampleId :
BFB630

m/z	Abundance
35.90	197.0
37.00	900.0
38.00	969.0
39.00	334.0
39.80	131.0
43.90	405.0
44.90	215.0
46.90	169.0
47.80	146.0
49.00	996.0
50.00	4279.0
51.00	1309.0
55.90	436.0
56.90	616.0
59.90	252.0
61.00	1069.0
61.90	1139.0
63.00	871.0
68.00	1985.0
69.00	2045.0
69.90	236.0
72.00	128.0
72.90	898.0
74.00	3753.0
75.00	10090.0
75.90	744.0
76.90	118.0
78.80	768.0
79.90	258.0
80.80	898.0
81.90	129.0
86.90	600.0
87.80	614.0
91.90	598.0
92.90	843.0
94.00	2459.0
95.00	17408.0
96.00	1040.0
105.80	125.0
116.80	101.0
118.80	128.0
128.00	112.0
140.80	280.0
142.80	222.0
173.90	16424.0
174.90	1165.0
175.90	15723.0
176.90	1104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB630

m/z	Abundance
43.90	189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB630