

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022322\
 Data File : VU047244.D
 Acq On : 23 Feb 2022 11:53
 Operator : SY/MD
 Sample : N1637-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB-01-022222

Quant Time: Feb 24 05:58:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Feb 15 03:17:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.118	96	49072	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.636	95	17290	0.910	ug/l	0.00
Spiked Amount	1.000		Recovery	=	91.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	18488	0.934	ug/l	0.00
Spiked Amount	1.000		Recovery	=	93.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022322\
Data File : VU047244.D
Acq On : 23 Feb 2022 11:53
Operator : SY/MD
Sample : N1637-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB-01-022222

Quant Time: Feb 24 05:58:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Feb 15 03:17:28 2022
Response via : Initial Calibration




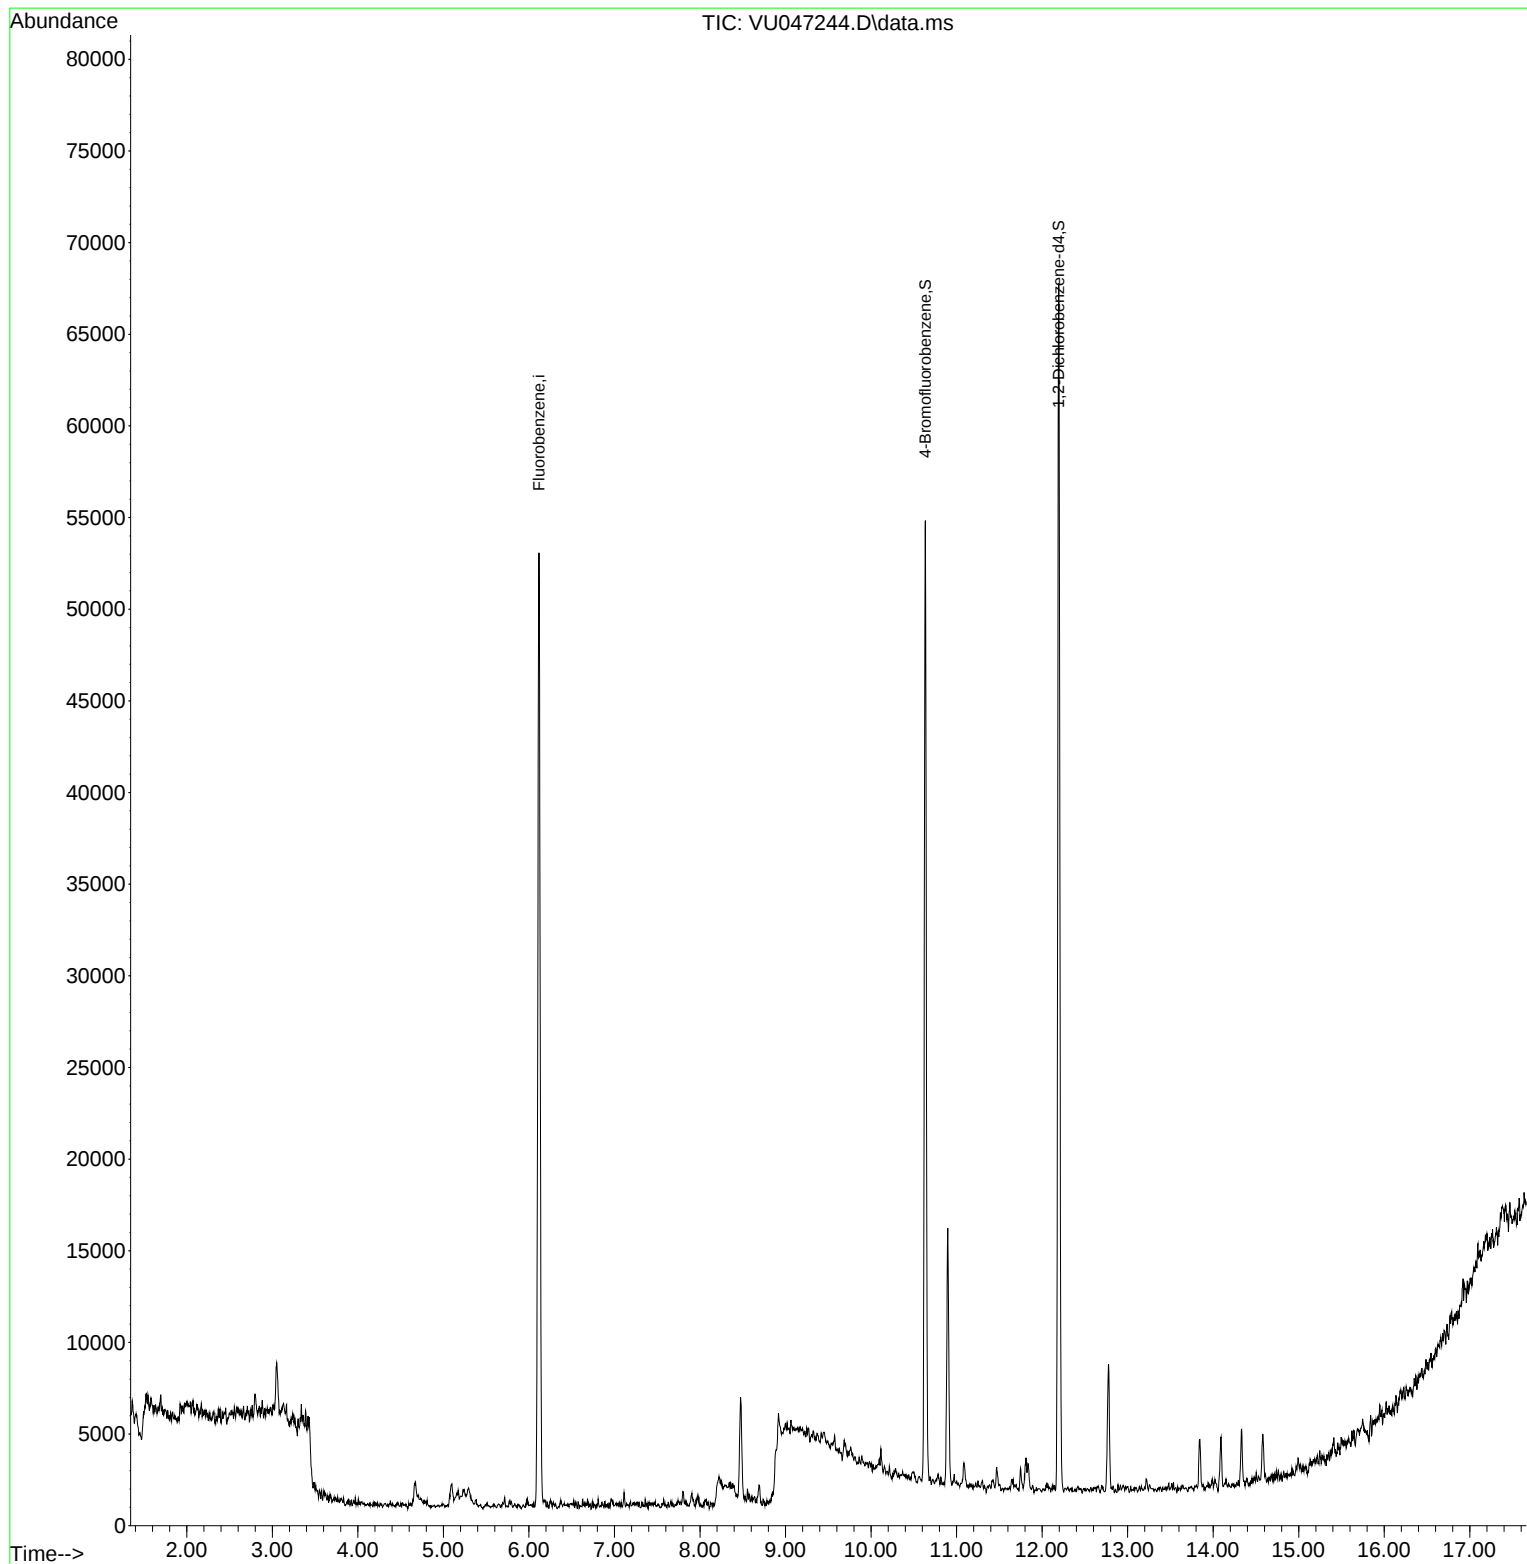


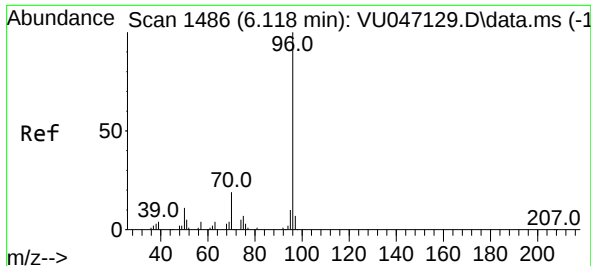

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.118 min Scan# 1486
Delta R.T. 0.000 min
Lab File: VU047244.D
Acq: 23 Feb 2022 11:53




Instrument :
MSVOA_U
ClientSampleId :
TB-01-022222


Tgt Ion: 96	Resp: 49072
Ion Ratio	Lower Upper
96 100	
70 19.1	16.8 25.2
95 9.5	7.3 10.9
97 6.7	0.0 0.0#

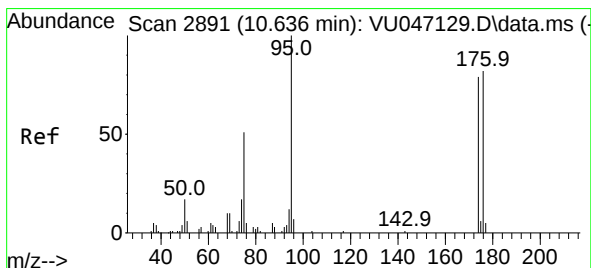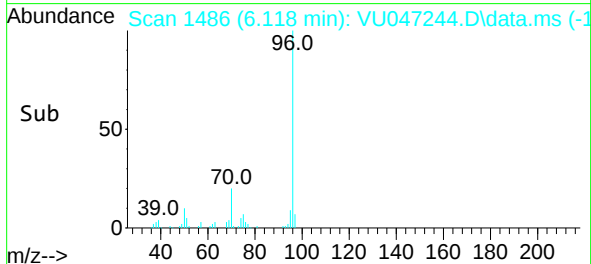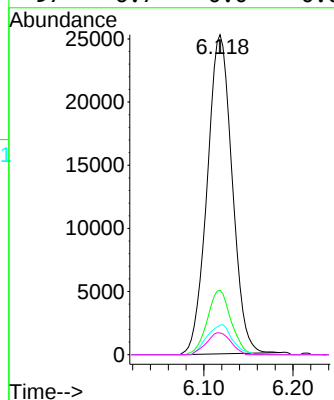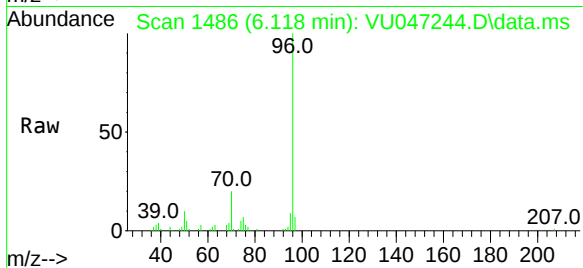

#57
4-Bromofluorobenzene
Concen: 0.910 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.000 min
Lab File: VU047244.D
Acq: 23 Feb 2022 11:53

Tgt Ion: 95	Resp: 17290
Ion Ratio	Lower Upper
95 100	
174 89.2	56.6 84.8#
176 84.1	54.3 81.5#

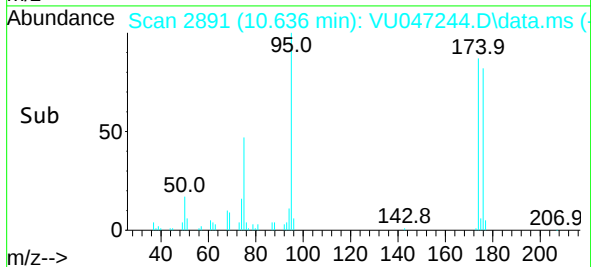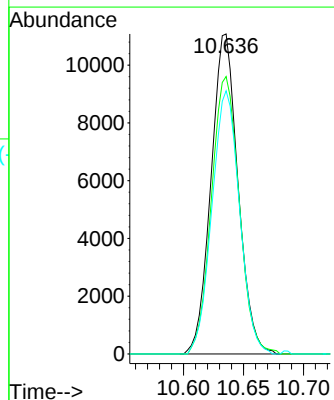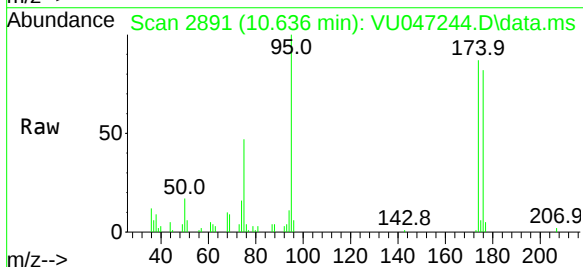

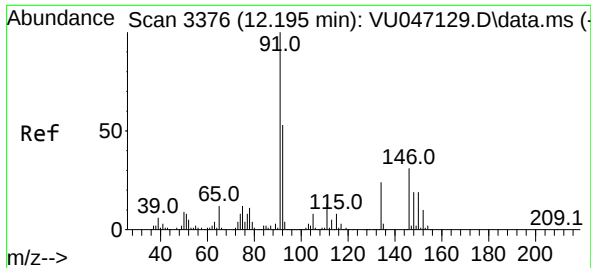

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.934 ug/l
 RT: 12.195 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: VU047244.D
 Acq: 23 Feb 2022 11:53

Instrument :
 MSVOA_U
 ClientSampleId :
 TB-01-022222

Tgt Ion:152	Resp:	18488
Ion Ratio	Lower	Upper
152	100	
115	62.3	0.0 251.0
150	159.4	0.0 613.8

