

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022322\
 Data File : VU047247.D
 Acq On : 23 Feb 2022 13:13
 Operator : SY/MD
 Sample : N1637-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PW-B6-L10-D-022222

Quant Time: Feb 24 05:59:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Feb 15 03:17:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.118	96	50708	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.636	95	17220	0.877	ug/l	0.00
Spiked Amount 1.000			Recovery	=	88.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	18321	0.896	ug/l	0.00
Spiked Amount 1.000			Recovery	=	90.000%	
Target Compounds						Qvalue
13) Acetone	2.639	43	6452	1.465	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022322\
Data File : VU047247.D
Acq On : 23 Feb 2022 13:13
Operator : SY/MD
Sample : N1637-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L10-D-022222

Quant Time: Feb 24 05:59:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Feb 15 03:17:28 2022
Response via : Initial Calibration




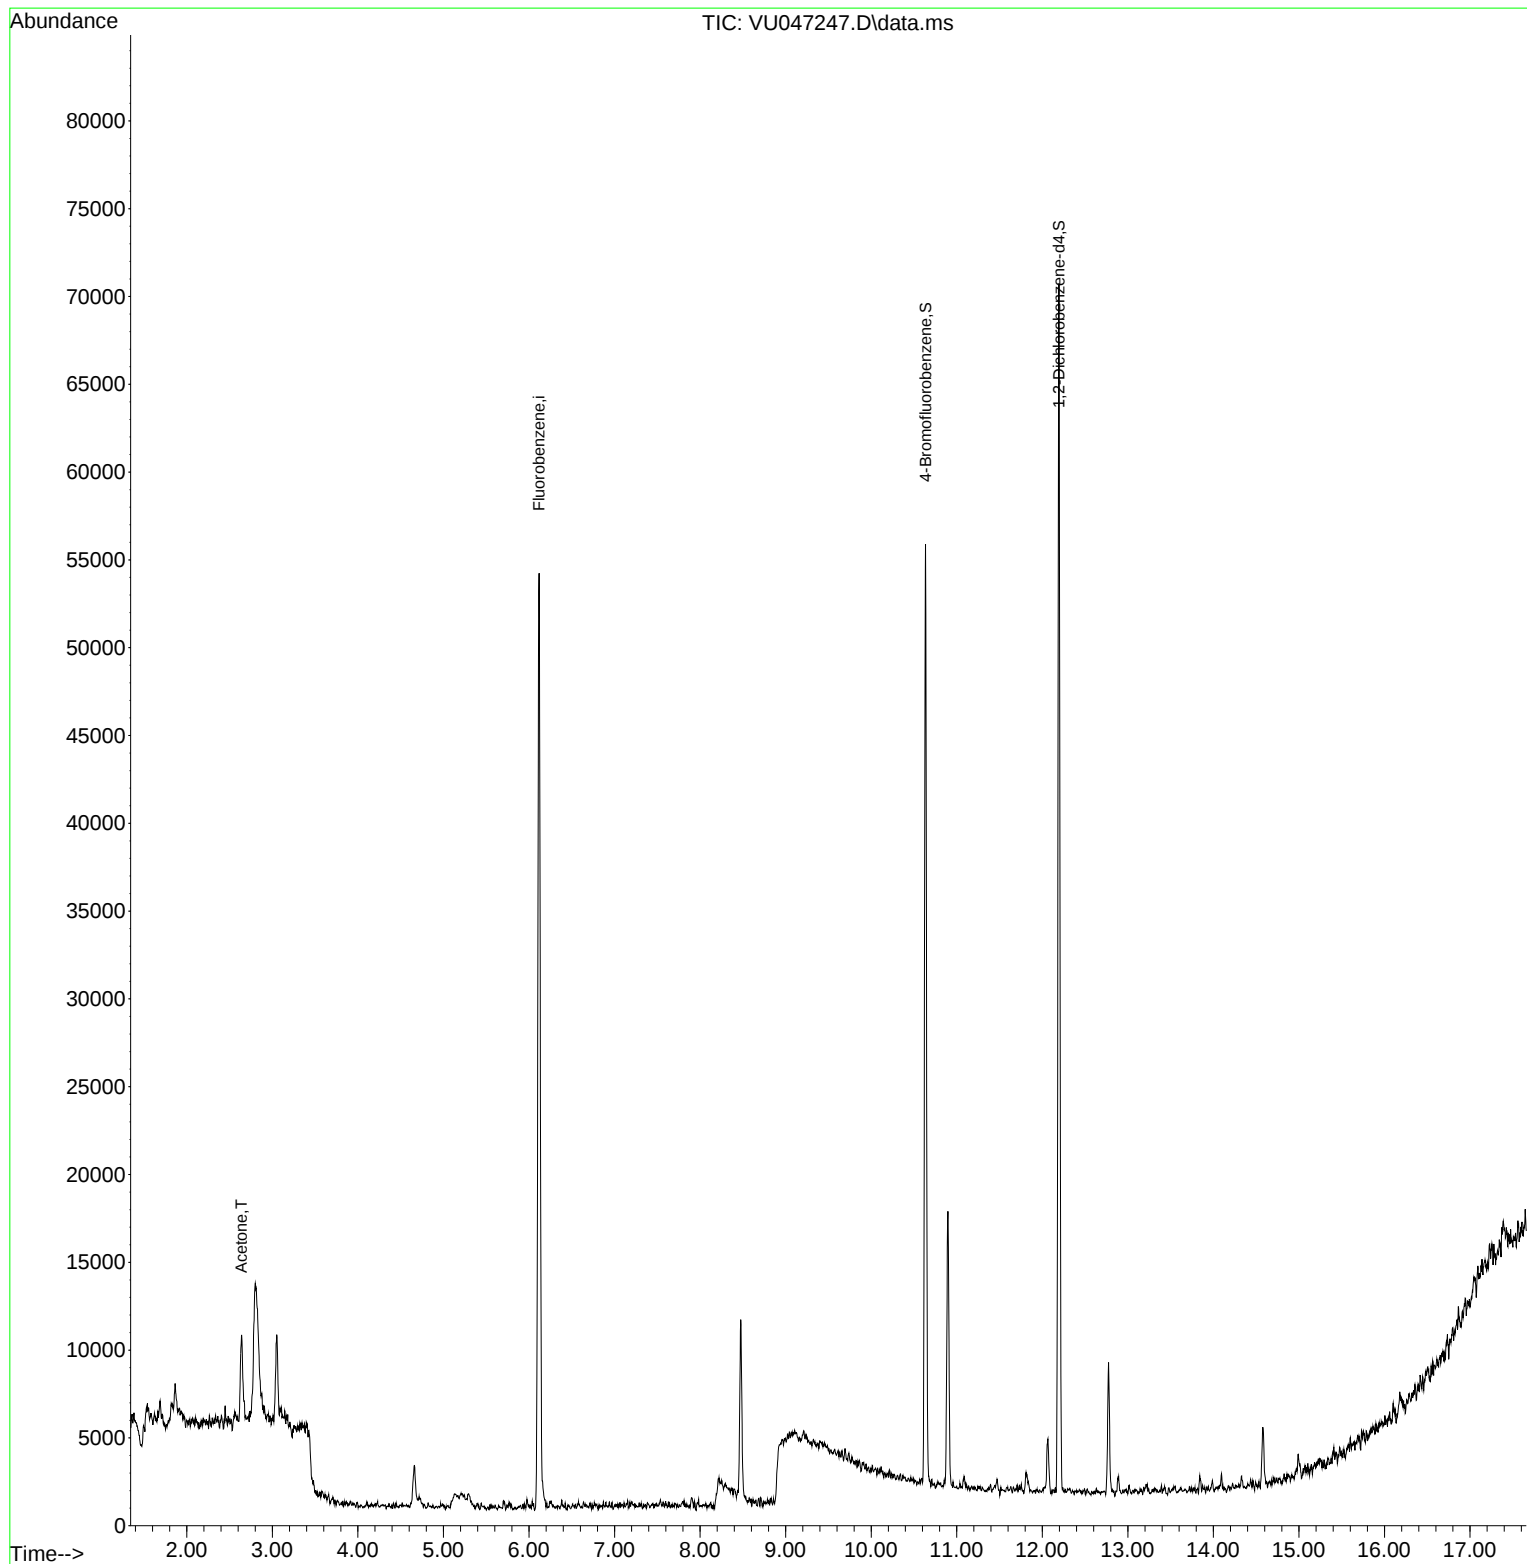


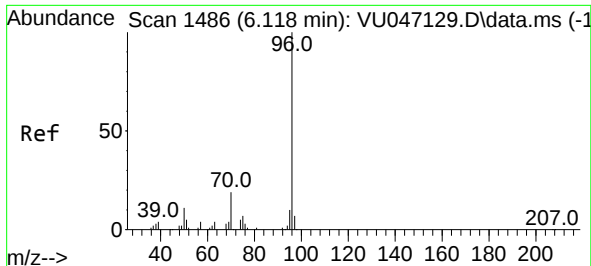

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.118 min Scan# 1486
Delta R.T. 0.000 min
Lab File: VU047247.D
Acq: 23 Feb 2022 13:13




Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L10-D-022222


Tgt Ion:	96	Resp:	50708
Ion	Ratio	Lower	Upper
96	100		
70	19.5	16.8	25.2
95	8.4	7.3	10.9
97	6.7	0.0	0.0

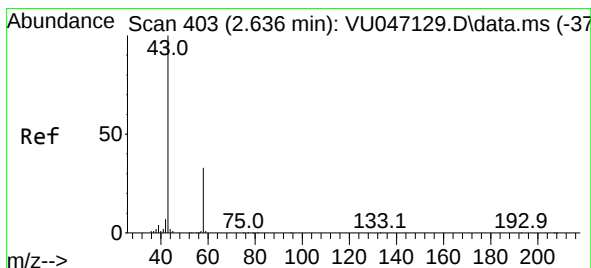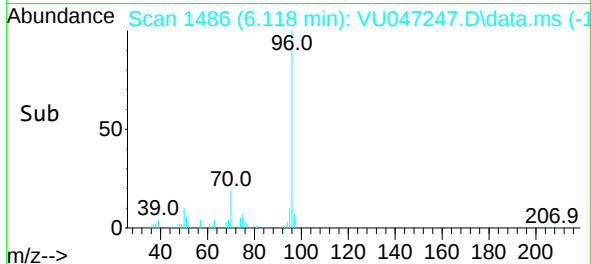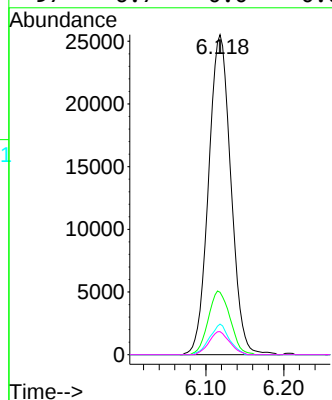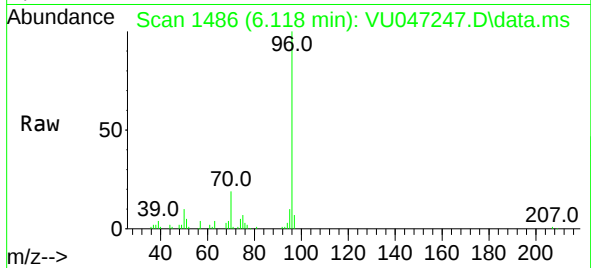

#13
Acetone
Concen: 1.465 ug/l
RT: 2.639 min Scan# 404
Delta R.T. 0.003 min
Lab File: VU047247.D
Acq: 23 Feb 2022 13:13

Tgt Ion:	43	Resp:	6452
Ion	Ratio	Lower	Upper
43	100		
58	33.5	27.1	40.7


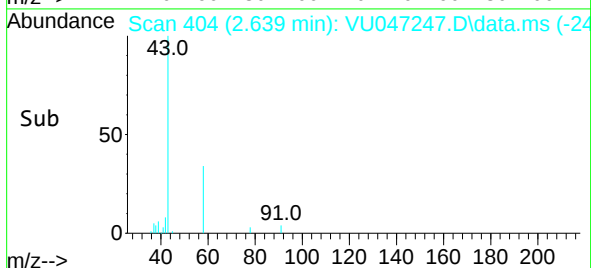
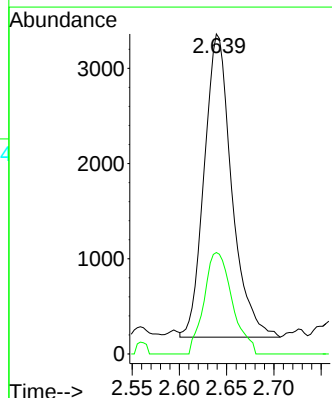
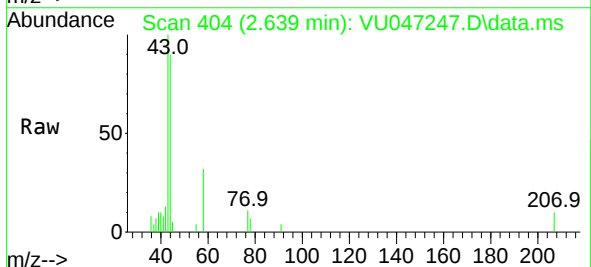


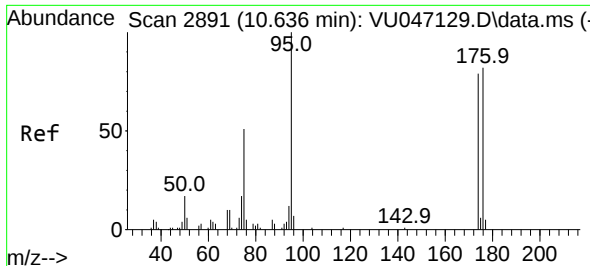

#57
4-Bromofluorobenzene
Concen: 0.877 ug/l
RT: 10.636 min Scan# 21
Delta R.T. 0.000 min
Lab File: VU047247.D
Acq: 23 Feb 2022 13:13

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L10-D-022222

Tgt Ion: 95 Resp: 17220
Ion Ratio Lower Upper
95 100
174 87.8 56.6 84.8#
176 84.8 54.3 81.5#

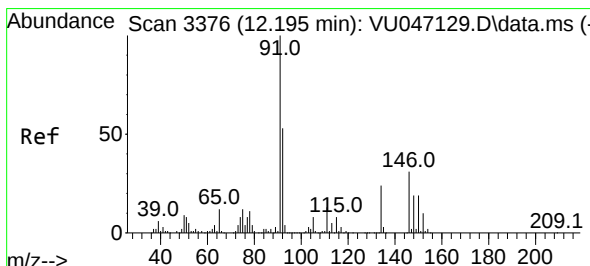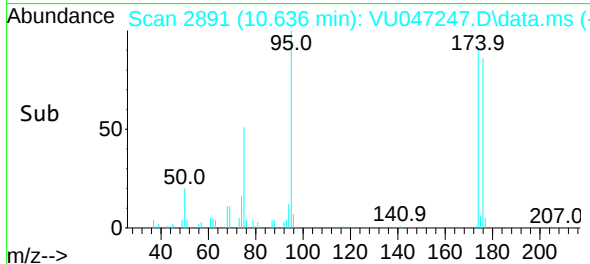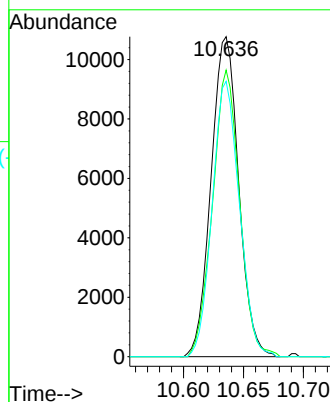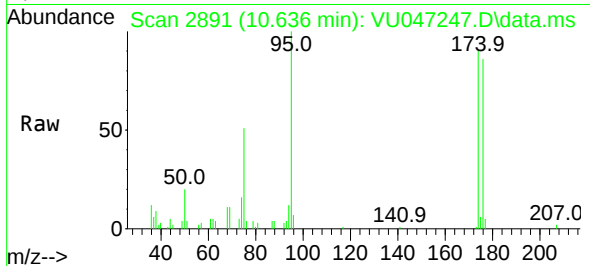

#68
1,2-Dichlorobenzene-d4
Concen: 0.896 ug/l
RT: 12.195 min Scan# 3376
Delta R.T. 0.000 min
Lab File: VU047247.D
Acq: 23 Feb 2022 13:13

Tgt Ion: 152 Resp: 18321
Ion Ratio Lower Upper
152 100
115 64.2 0.0 251.0
150 162.4 0.0 613.8

