

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022322\
 Data File : VU047248.D
 Acq On : 23 Feb 2022 13:41
 Operator : SY/MD
 Sample : N1637-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PW-B6-L10-D-022222-FD

Quant Time: Feb 24 05:59:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Feb 15 03:17:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.118	96	49217	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.632	95	17171	0.901	ug/l	0.00
Spiked Amount 1.000			Recovery	=	90.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	18649	0.939	ug/l	0.00
Spiked Amount 1.000			Recovery	=	94.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022322\
Data File : VU047248.D
Acq On : 23 Feb 2022 13:41
Operator : SY/MD
Sample : N1637-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L10-D-022222-FD

Quant Time: Feb 24 05:59:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Feb 15 03:17:28 2022
Response via : Initial Calibration




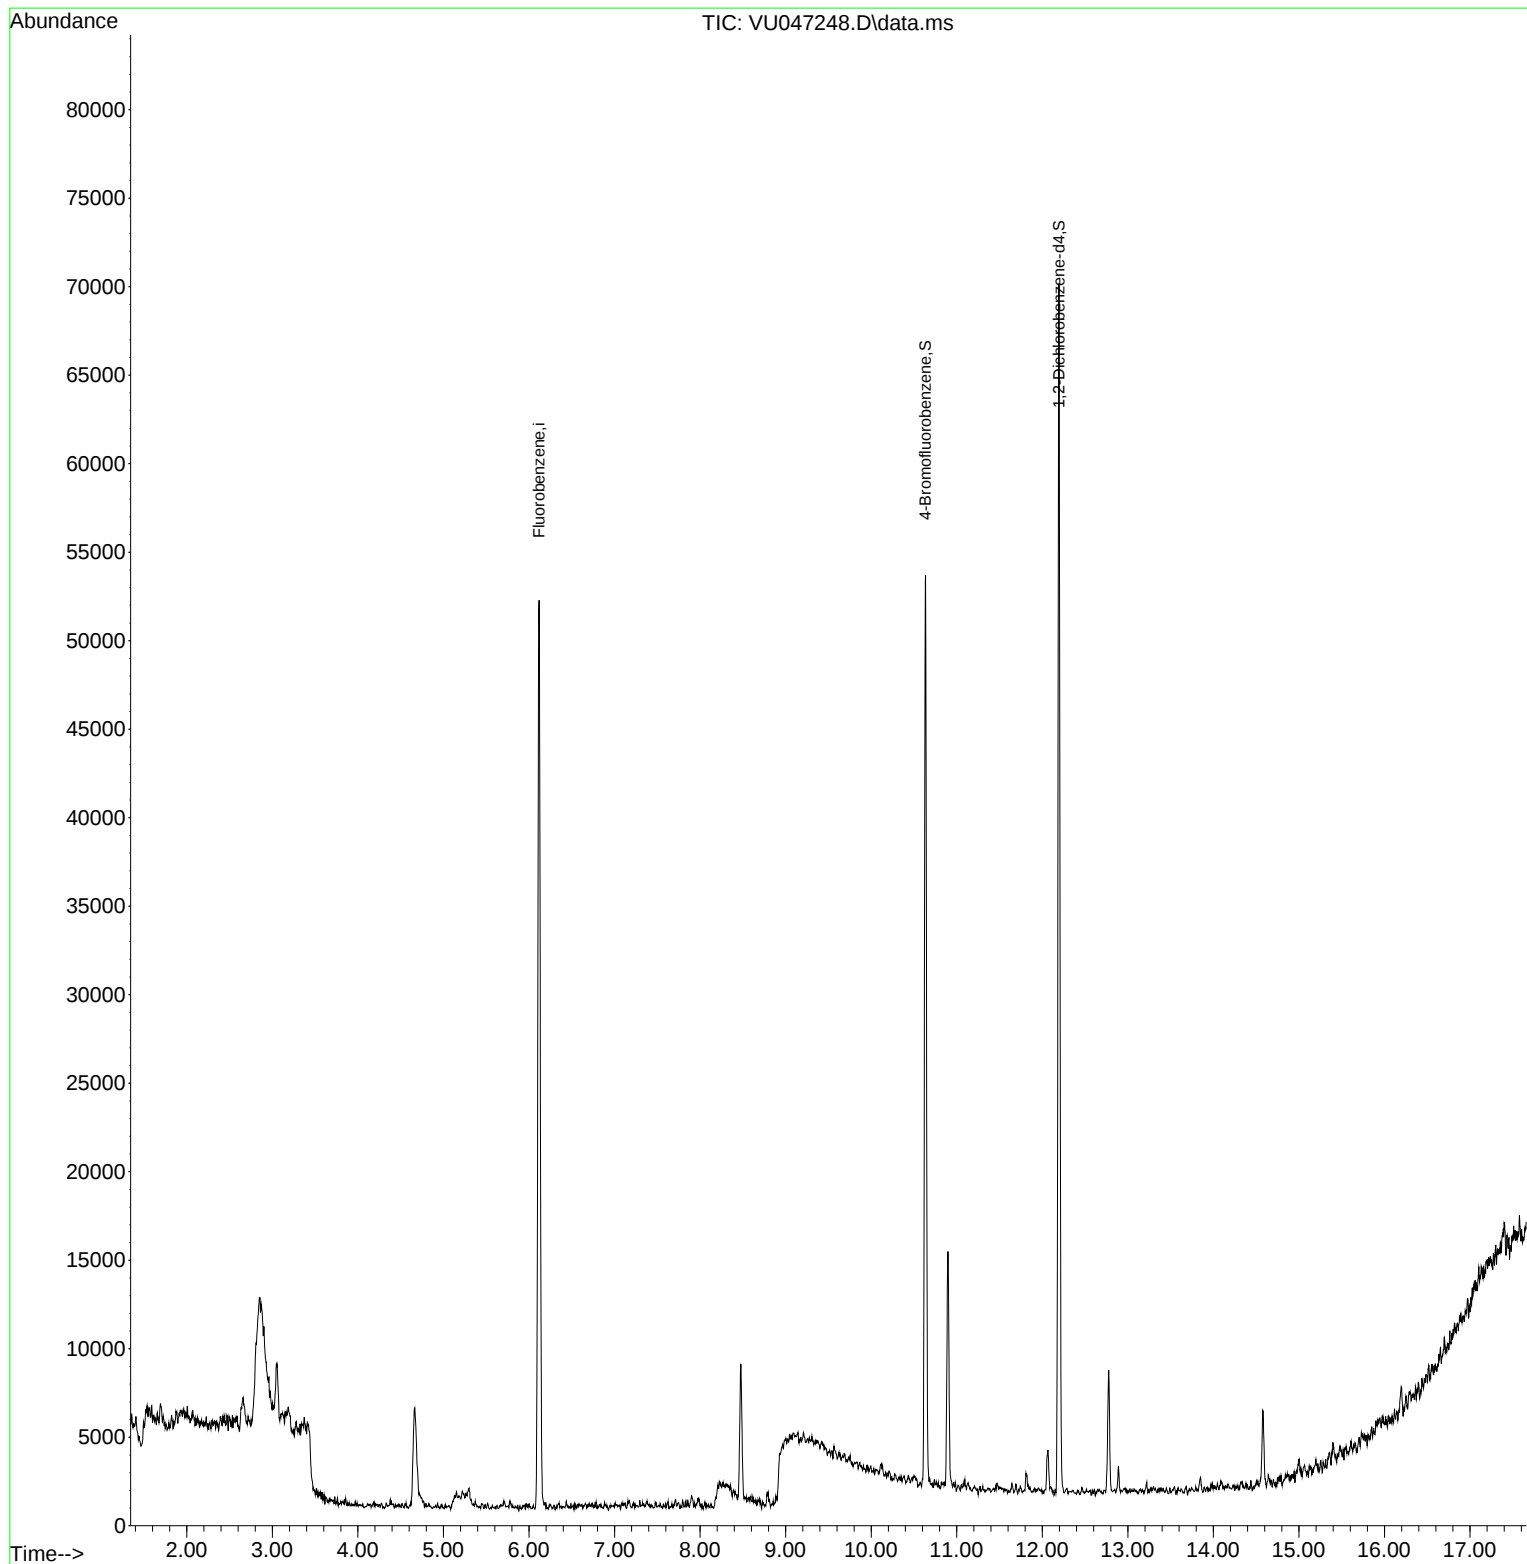


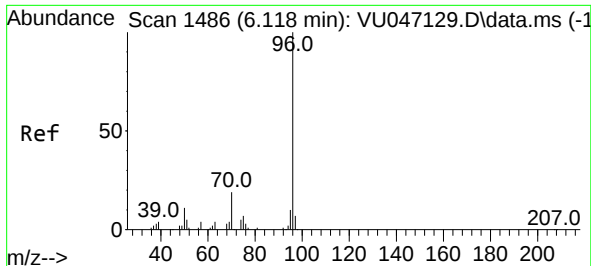

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.118 min Scan# 1486
Delta R.T. -0.000 min
Lab File: VU047248.D
Acq: 23 Feb 2022 13:41




Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L10-D-022222-FD


Tgt Ion:	96	Resp:	49217
Ion Ratio	Lower	Upper	
96	100		
70	18.8	16.8	25.2
95	8.8	7.3	10.9
97	6.6	0.0	0.0#

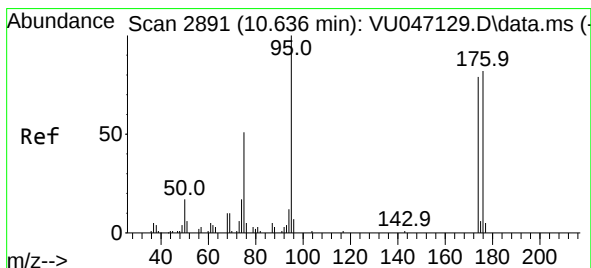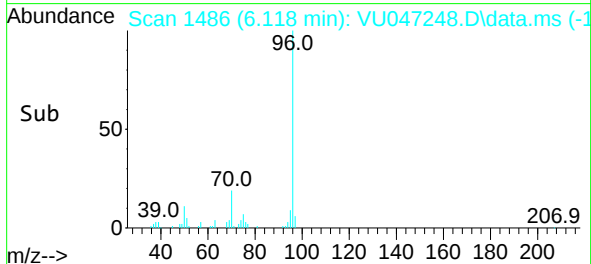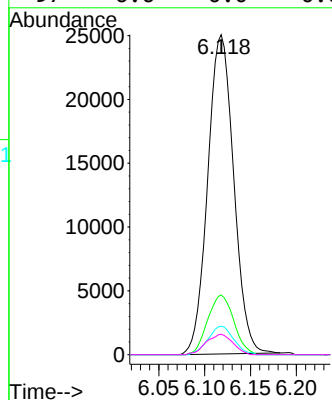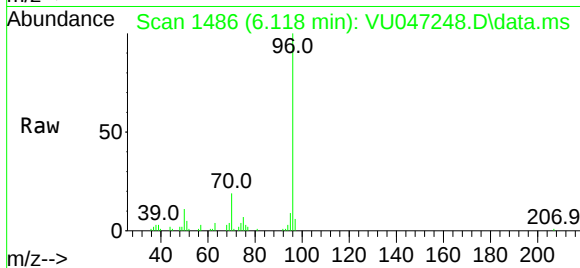

#57
4-Bromofluorobenzene
Concen: 0.901 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. -0.003 min
Lab File: VU047248.D
Acq: 23 Feb 2022 13:41


Tgt Ion:	95	Resp:	17171
Ion Ratio	Lower	Upper	
95	100		
174	88.0	56.6	84.8#
176	83.7	54.3	81.5#

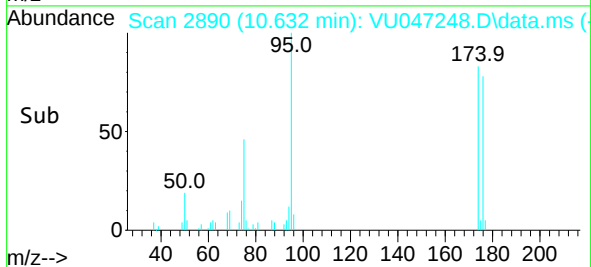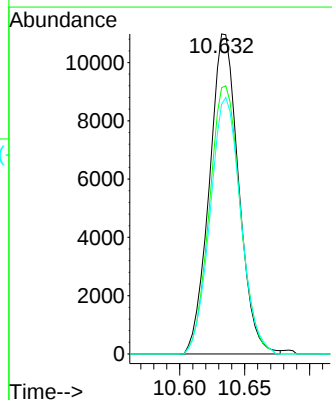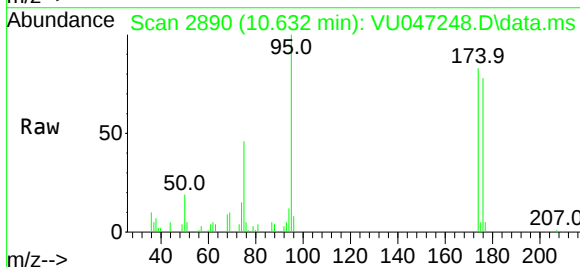

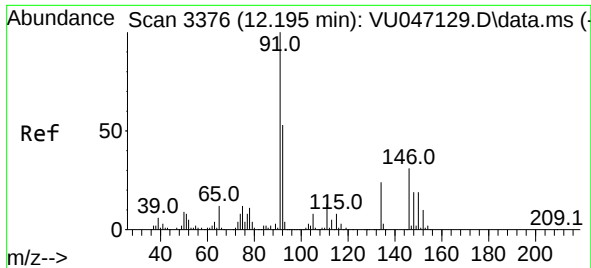

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.939 ug/l
 RT: 12.195 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VU047248.D
 Acq: 23 Feb 2022 13:41

Instrument :
 MSVOA_U
 ClientSampleId :
 PW-B6-L10-D-022222-FD

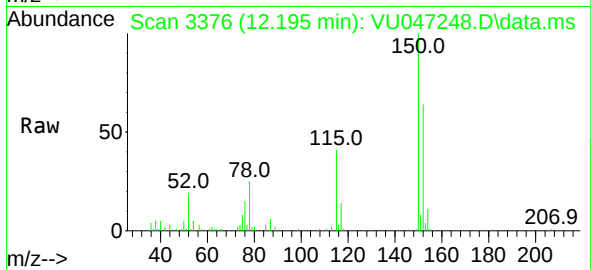

Tgt Ion:	152	Resp:	18649
Ion Ratio	Lower	Upper	
152	100		
115	63.1	0.0	251.0
150	158.3	0.0	613.8

