

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022322\
 Data File : VU047246.D
 Acq On : 23 Feb 2022 12:46
 Operator : SY/MD
 Sample : N1637-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PW-B6-L10-M-022222

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU047246.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.047	525	531	542	rVB2	6775	11731	10.97%	3.292%
2	4.668	1021	1035	1044	rBV2	1700	4242	3.97%	1.190%
3	5.292	1225	1229	1238	rVB5	715	1197	1.12%	0.336%
4	6.118	1470	1486	1514	rBV	53216	106913	100.00%	30.003%
5	8.205	2125	2135	2136	rBV3	1514	1776	1.66%	0.498%
6	8.475	2209	2219	2234	rVB2	6021	11108	10.39%	3.117%
7	8.938	2348	2363	2364	rBV6	2893	5244	4.90%	1.472%
8	10.346	2796	2801	2807	rVB5	1433	1612	1.51%	0.452%
9	10.636	2880	2891	2905	rVB	51606	80672	75.46%	22.639%
10	10.893	2963	2971	2987	rVB3	9411	16405	15.34%	4.604%
11	11.816	3250	3258	3263	rBV6	1111	1843	1.72%	0.517%
12	12.063	3327	3335	3343	rBV3	2175	3590	3.36%	1.007%
13	12.195	3364	3376	3392	rBV	59114	97272	90.98%	27.298%
14	12.777	3547	3557	3570	rBV2	3378	5498	5.14%	1.543%
15	14.584	4110	4119	4126	rBB	3180	5124	4.79%	1.438%
16	15.413	4369	4377	4385	rBV9	1216	2110	1.97%	0.592%




Sum of corrected areas: 356337

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022322\
Data File : VU047246.D
Acq On : 23 Feb 2022 12:46
Operator : SY/MD
Sample : N1637-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L10-M-022222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

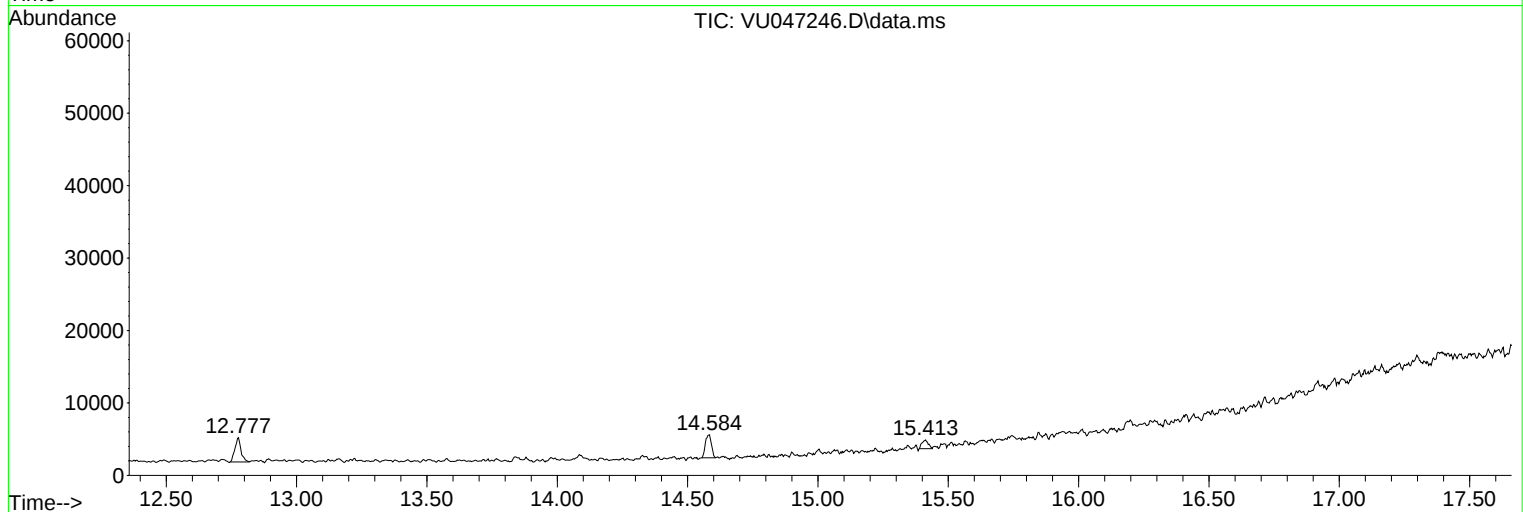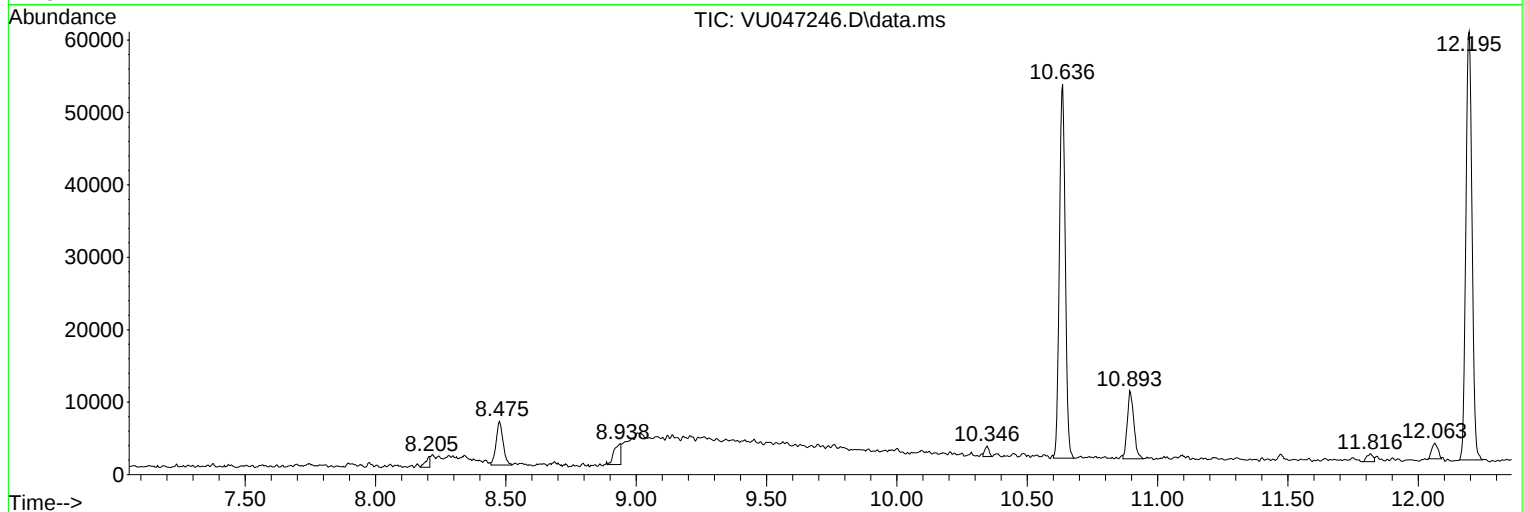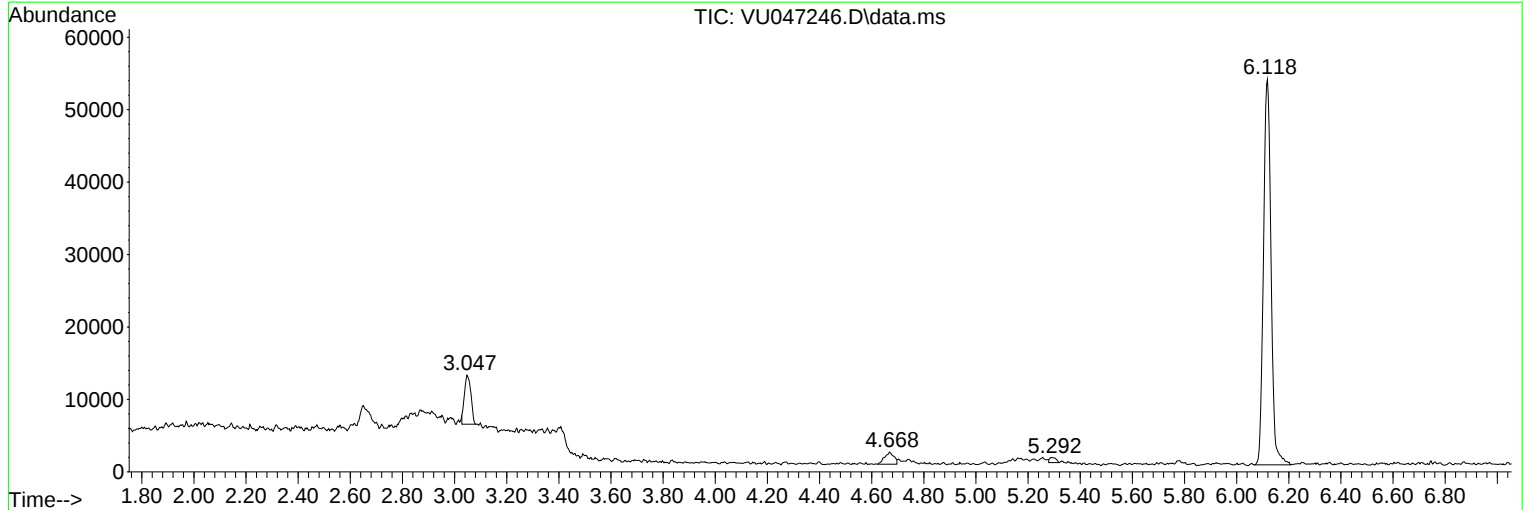

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022322\
Data File : VU047246.D
Acq On : 23 Feb 2022 12:46
Operator : SY/MD
Sample : N1637-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L10-M-022222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022322\
Data File : VU047246.D
Acq On : 23 Feb 2022 12:46
Operator : SY/MD
Sample : N1637-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L10-M-022222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------