

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022322\
 Data File : VU047248.D
 Acq On : 23 Feb 2022 13:41
 Operator : SY/MD
 Sample : N1637-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PW-B6-L10-D-022222-FD

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU047248.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.809	452	457	458	rBV5	2387	2148	1.98%	0.573%
2	4.665	1019	1034	1051	rBV2	5555	16568	15.24%	4.421%
3	6.118	1470	1486	1504	rBV	51346	101051	92.98%	26.962%
4	7.899	2033	2040	2048	rBV3	676	1107	1.02%	0.295%
5	8.475	2207	2219	2231	rBV2	7689	13882	12.77%	3.704%
6	8.931	2352	2361	2362	rBV3	2611	3209	2.95%	0.856%
7	10.635	2881	2891	2904	rVB2	51212	81251	74.76%	21.679%
8	10.896	2962	2972	2989	rVB2	13306	22598	20.79%	6.030%
9	12.066	3328	3336	3343	rBV5	2244	3567	3.28%	0.952%
10	12.195	3365	3376	3395	rBV	68337	108685	100.00%	28.999%
11	12.777	3546	3557	3566	rBV	6908	10777	9.92%	2.876%
12	12.889	3587	3592	3600	rVB3	1510	1640	1.51%	0.438%
13	13.848	3882	3890	3899	rVB5	852	1357	1.25%	0.362%
14	14.577	4109	4117	4125	rBV	3929	5795	5.33%	1.546%
15	14.642	4130	4137	4145	rBV5	719	1149	1.06%	0.307%




Sum of corrected areas: 374784

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022322\
Data File : VU047248.D
Acq On : 23 Feb 2022 13:41
Operator : SY/MD
Sample : N1637-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L10-D-022222-FD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

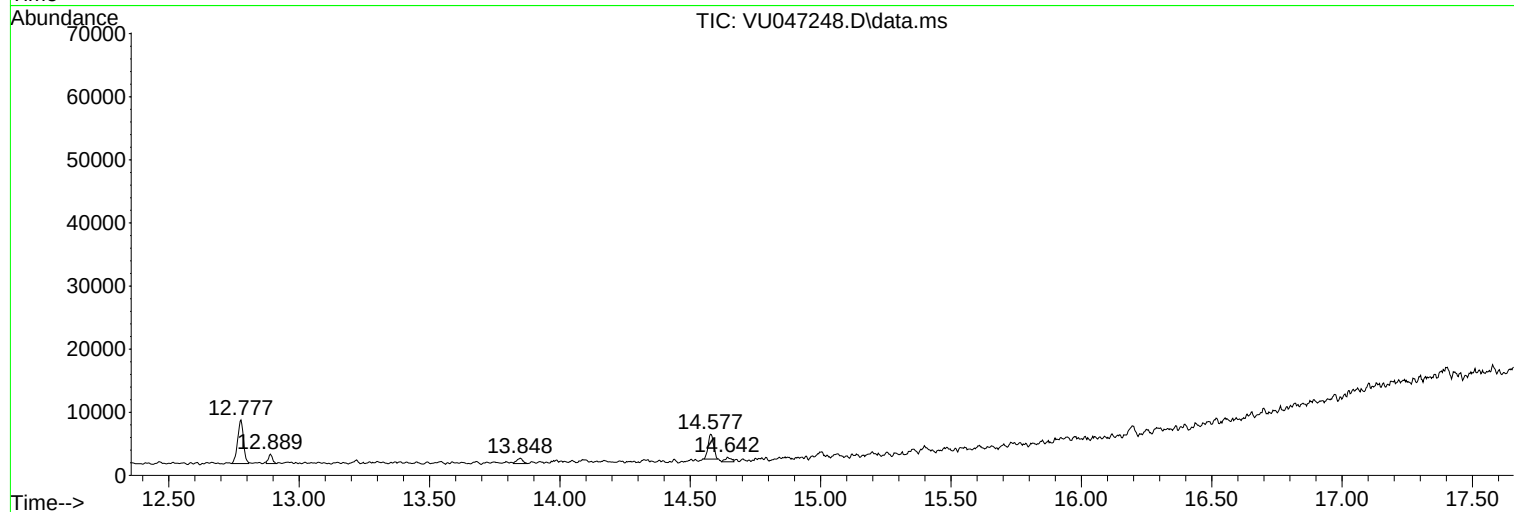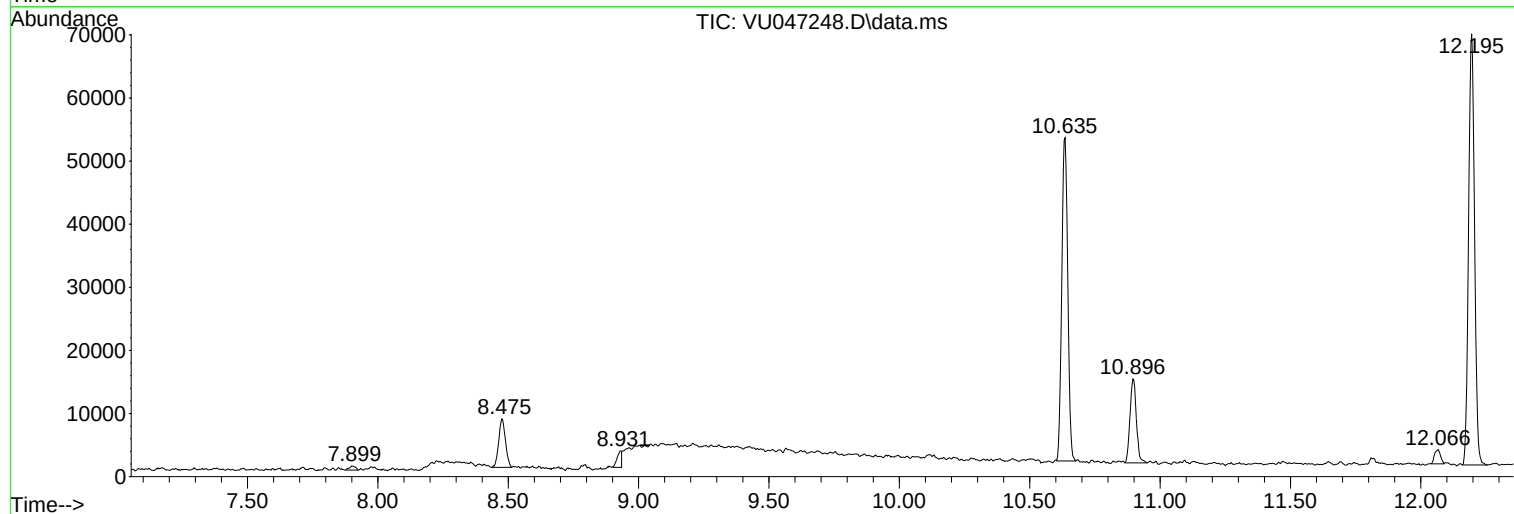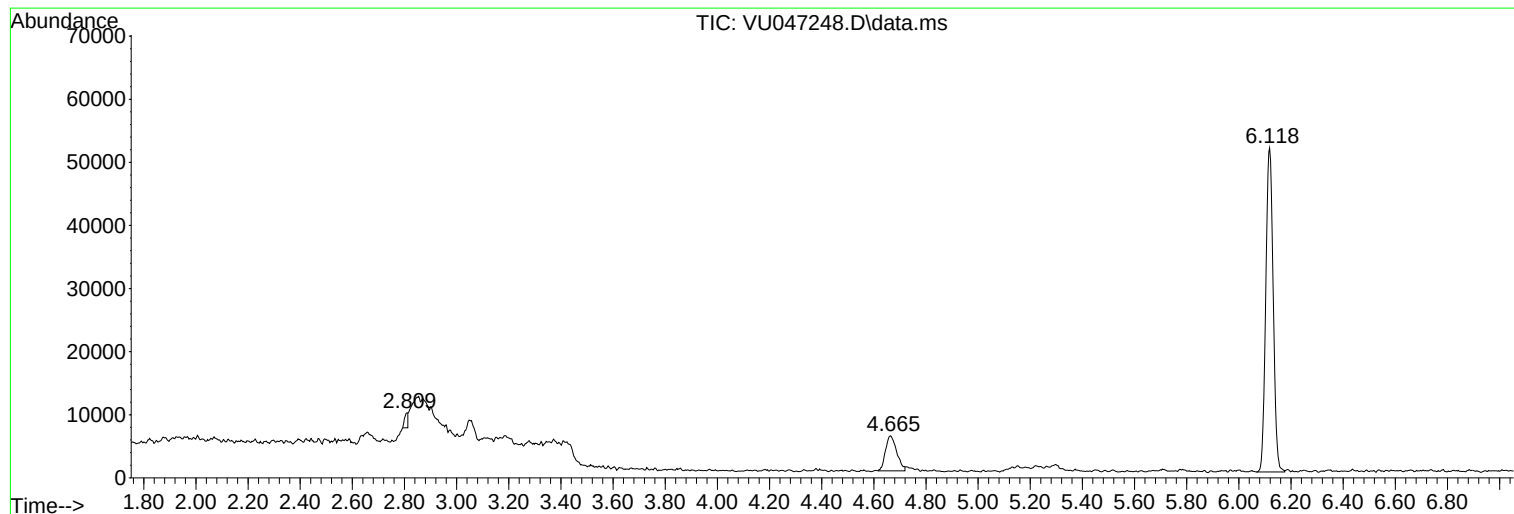

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022322\
Data File : VU047248.D
Acq On : 23 Feb 2022 13:41
Operator : SY/MD
Sample : N1637-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L10-D-022222-FD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022322\
Data File : VU047248.D
Acq On : 23 Feb 2022 13:41
Operator : SY/MD
Sample : N1637-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L10-D-022222-FD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------