


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU022420\
 Data File : VU036877.D
 Acq On : 24 Feb 2020 11:25
 Operator : JC/MD
 Sample : BFB50
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB50

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis
 Last Update : Tue Feb 25 03:18:14 2020

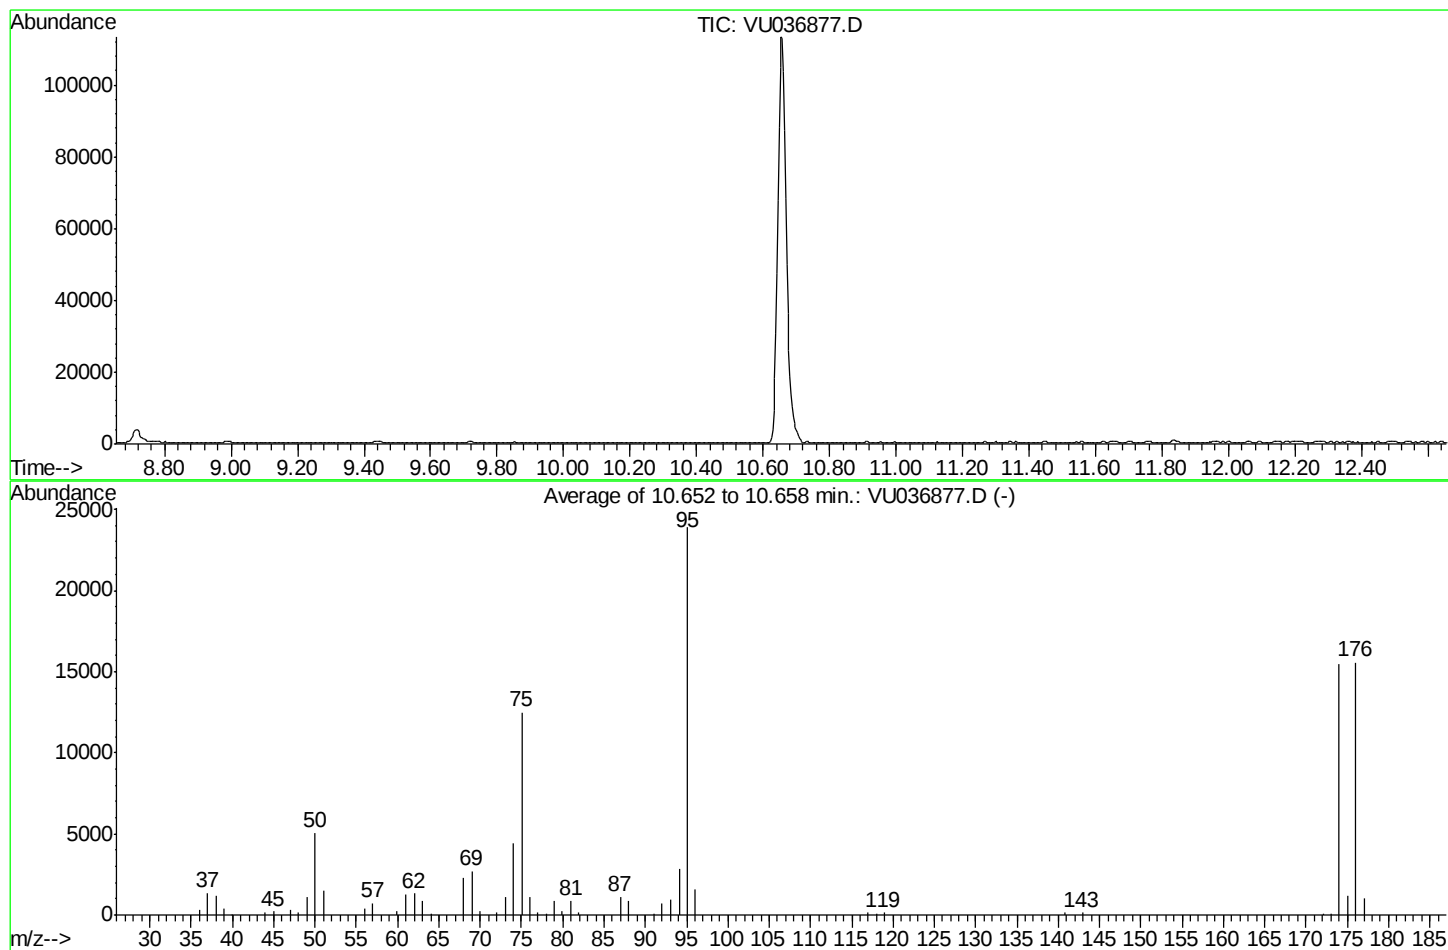

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	5065	PASS
75	95	30	80	52.2	12475	PASS
95	95	100	100	100.0	23893	PASS
96	95	5	9	6.5	1559	PASS
173	174	0.00	2	0.7	106	PASS
174	95	50	120	64.8	15480	PASS
175	174	5	9	7.8	1204	PASS
176	174	95	101	100.5	15559	PASS
177	176	5	9	6.7	1040	PASS

m/z	Abundance
35.90	317.0
37.00	1381.0
38.00	1144.0
38.90	369.0
40.00	162.0
43.90	483.0
45.00	207.0
46.90	325.0
48.00	174.0
49.00	1149.0
50.00	4965.0
51.00	1441.0
56.00	409.0
57.00	705.0
59.90	210.0
61.00	1256.0
62.00	1276.0
63.00	885.0
64.00	112.0
68.00	2177.0
69.00	2637.0
70.00	213.0
72.00	127.0
73.00	986.0
74.10	4119.0
75.00	11973.0
76.10	1101.0
76.90	147.0
78.90	898.0
79.90	251.0
81.00	894.0
81.80	185.0
86.90	1097.0
88.00	824.0
91.00	107.0
92.00	678.0
93.00	974.0
94.10	2700.0
95.10	22592.0
96.00	1431.0
117.10	114.0
117.90	121.0
118.90	120.0
140.90	123.0
143.00	139.0
172.30	101.0
174.00	14564.0
175.00	1123.0
176.00	14319.0
177.00	981.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
35.00	311.0
37.00	1434.0
38.00	1223.0
39.00	412.0
40.00	160.0
43.90	532.0
45.00	231.0
46.90	312.0
48.00	202.0
49.00	1144.0
50.00	5217.0
51.00	1582.0
56.00	449.0
57.00	767.0
60.00	213.0
61.00	1327.0
62.00	1344.0
63.00	854.0
64.00	114.0
68.00	2320.0
69.00	2775.0
70.00	238.0
72.00	146.0
73.00	1164.0
74.00	4546.0
75.00	12837.0
76.00	1149.0
77.00	177.0
79.00	888.0
79.90	260.0
81.00	935.0
81.90	179.0
86.90	1162.0
88.00	841.0
91.00	115.0
92.00	720.0
93.00	1013.0
94.10	2879.0
95.10	24592.0
96.10	1579.0
116.90	136.0
118.00	119.0
118.90	156.0
140.80	137.0
142.90	138.0
172.10	114.0
174.00	15883.0
175.00	1187.0
176.00	16127.0
177.00	1053.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
36.00	261.0
37.00	1331.0
38.00	1231.0
38.90	487.0
40.00	158.0
43.90	529.0
45.00	241.0
47.00	283.0
47.90	189.0
49.00	1084.0
50.00	5013.0
51.00	1541.0
56.00	431.0
57.00	735.0
60.00	216.0
61.00	1315.0
62.00	1312.0
63.00	902.0
64.00	113.0
68.00	2307.0
69.00	2713.0
70.00	230.0
71.90	161.0
73.00	1206.0
74.00	4603.0
75.10	12616.0
76.00	1061.0
77.00	209.0
78.00	135.0
78.90	808.0
79.90	252.0
81.00	890.0
81.90	147.0
87.00	1129.0
87.90	911.0
91.00	100.0
92.00	707.0
93.00	940.0
94.10	2871.0
95.10	24496.0
96.10	1669.0
116.90	174.0
118.90	172.0
140.80	129.0
143.00	140.0
172.00	118.0
173.10	319.0
174.00	15993.0
175.00	1303.0
176.00	16231.0
177.00	1088.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

Scan 2885 (10.616 min): VU036877.D
BFB50

m/z	Abundance
39.90	133.0
44.00	330.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50