

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022421\
 Data File : VU042419.D
 Acq On : 24 Feb 2021 10:29
 Operator : SY/MD
 Sample : VU0224WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK113

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M

Title : VOC Analysis

Signal : TIC: VU042419.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	97	rVB	100576	118975	12.64%	1.647%
2	1.916	172	179	194	rVB	87772	114346	12.15%	1.583%
3	2.575	371	384	406	rBV	201163	346083	36.77%	4.791%
4	2.704	421	424	426	rBV	237	150	0.02%	0.002%
5	2.958	499	503	506	rBV2	246	241	0.03%	0.003%
6	3.196	575	577	581	rBV	139	111	0.01%	0.002%
7	3.241	588	591	593	rBV2	185	128	0.01%	0.002%
8	3.353	621	626	628	rBV	207	170	0.02%	0.002%
9	3.440	652	653	654	rBB	57	26	0.00%	0.000%
10	3.488	665	668	670	rBV	200	109	0.01%	0.002%
11	3.598	700	702	704	rBV	147	59	0.01%	0.001%
12	3.614	705	707	709	rVB	168	70	0.01%	0.001%
13	3.977	816	820	825	rBV2	260	318	0.03%	0.004%
14	4.028	833	836	839	rBV	175	95	0.01%	0.001%
15	4.073	848	850	852	rVB	116	42	0.00%	0.001%
16	4.318	923	926	927	rBV	155	68	0.01%	0.001%
17	4.469	969	973	976	rBV2	220	172	0.02%	0.002%
18	4.639	1011	1026	1059	rBV2	96900	265540	28.21%	3.676%
19	4.967	1126	1128	1130	rVB	224	91	0.01%	0.001%
20	4.987	1130	1134	1136	rBV2	199	153	0.02%	0.002%
21	5.073	1144	1161	1181	rBV	175428	380221	40.40%	5.264%
22	5.205	1200	1202	1206	rBV	261	200	0.02%	0.003%
23	5.282	1224	1226	1227	rBV	411	183	0.02%	0.003%
24	5.353	1245	1248	1251	rBV	211	161	0.02%	0.002%
25	5.546	1304	1308	1311	rVB2	273	234	0.02%	0.003%
26	5.565	1311	1314	1318	rVB	103	78	0.01%	0.001%
27	5.588	1319	1321	1322	rBV	152	46	0.00%	0.001%
28	5.736	1345	1367	1386	rBV2	345227	941168	100.00%	13.030%
29	5.954	1432	1435	1438	rVV	251	174	0.02%	0.002%
30	5.977	1439	1442	1446	rVB3	278	222	0.02%	0.003%
31	6.060	1463	1468	1475	rBV3	303	498	0.05%	0.007%
32	6.112	1481	1484	1487	rBV	284	204	0.02%	0.003%
33	6.257	1514	1529	1551	rBV	269927	514717	54.69%	7.126%
34	6.469	1591	1595	1598	rBV	295	294	0.03%	0.004%
35	6.536	1607	1616	1625	rBV5	2697	4613	0.49%	0.064%
36	6.642	1645	1649	1652	rBV	335	287	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022421\
 Data File : VU042419.D
 Acq On : 24 Feb 2021 10:29
 Operator : SY/MD
 Sample : VU0224WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK113

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
 Title : VOC Analysis

37	6.700	1652	1667	1690	rVV	226038	434113	46.12%	6.010%
38	6.900	1727	1729	1731	rBV	172	116	0.01%	0.002%
39	7.189	1813	1819	1823	rBV3	489	524	0.06%	0.007%
40	7.276	1845	1846	1847	rBV3	100	19	0.00%	0.000%
41	7.575	1925	1939	1957	rBV	132408	233739	24.83%	3.236%
42	7.748	1991	1993	1996	rBV	131	91	0.01%	0.001%
43	7.906	2025	2042	2061	rBV	421625	732465	77.83%	10.140%
44	8.189	2117	2130	2145	rBV	92190	160361	17.04%	2.220%
45	8.646	2258	2272	2298	rBV	329706	594539	63.17%	8.231%
46	8.806	2320	2322	2328	rVB	302	288	0.03%	0.004%
47	8.835	2328	2331	2336	rVB	235	141	0.01%	0.002%
48	9.067	2400	2403	2407	rBV	214	201	0.02%	0.003%
49	9.221	2446	2451	2454	rBV	236	219	0.02%	0.003%
50	9.424	2501	2514	2535	rBV	370885	620582	65.94%	8.591%
51	9.700	2594	2600	2609	rBV3	595	1022	0.11%	0.014%
52	10.469	2836	2839	2842	rBV	210	156	0.02%	0.002%
53	10.764	2919	2931	2949	rVB	298336	482525	51.27%	6.680%
54	10.986	2996	3000	3003	rBV	229	178	0.02%	0.002%
55	11.092	3030	3033	3038	rBV	384	479	0.05%	0.007%
56	11.752	3235	3238	3247	rVB2	944	869	0.09%	0.012%
57	11.819	3247	3259	3278	rBV	374630	599184	63.66%	8.295%
58	12.202	3365	3378	3393	rBV	414459	670843	71.28%	9.287%
59	12.819	3567	3570	3572	rBV	274	180	0.02%	0.002%
60	13.006	3626	3628	3630	rBV	385	185	0.02%	0.003%




Sum of corrected areas: 7223266

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022421\
Data File : VU042419.D
Acq On : 24 Feb 2021 10:29
Operator : SY/MD
Sample : VU0224WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

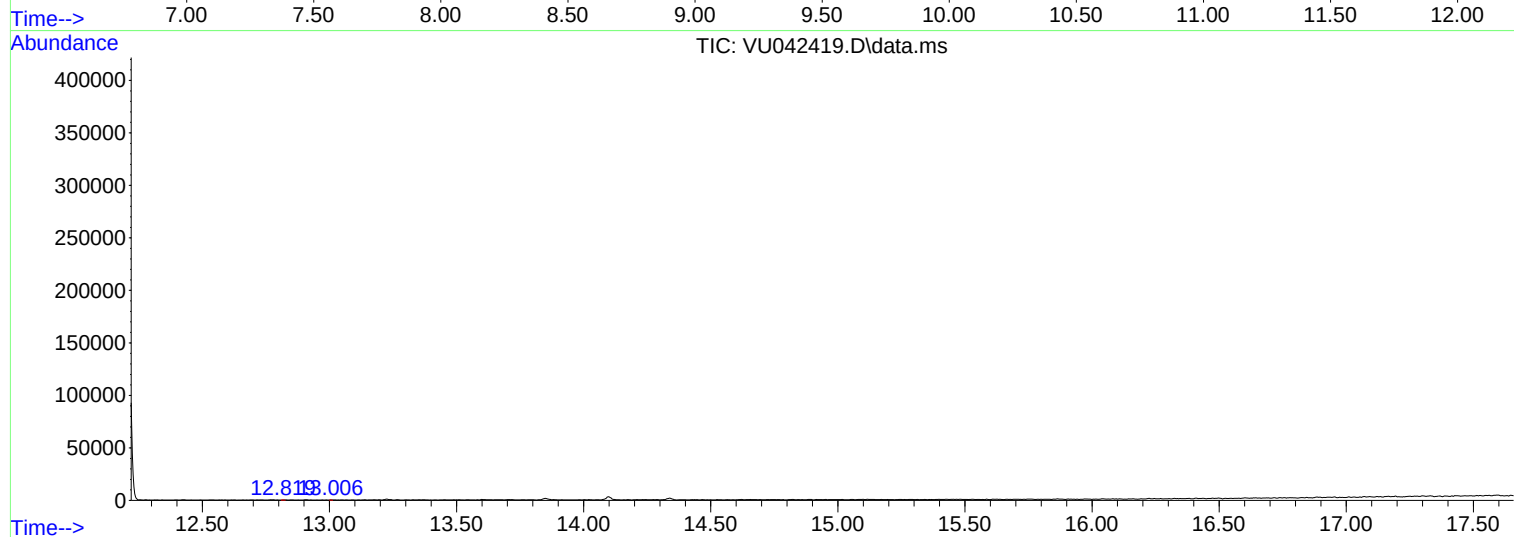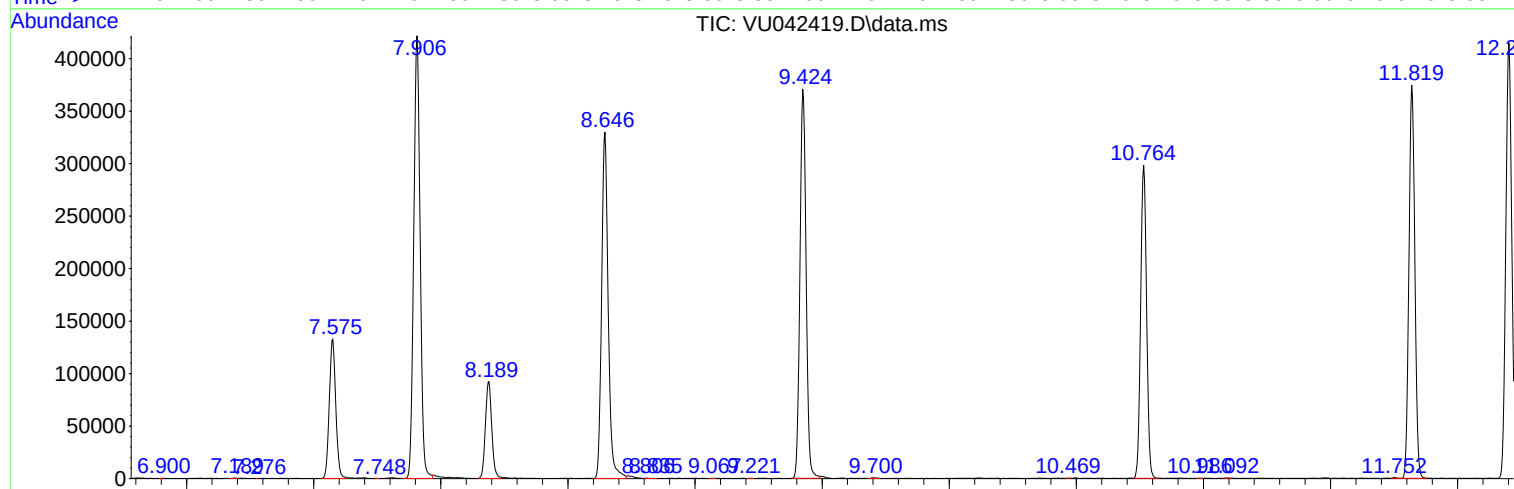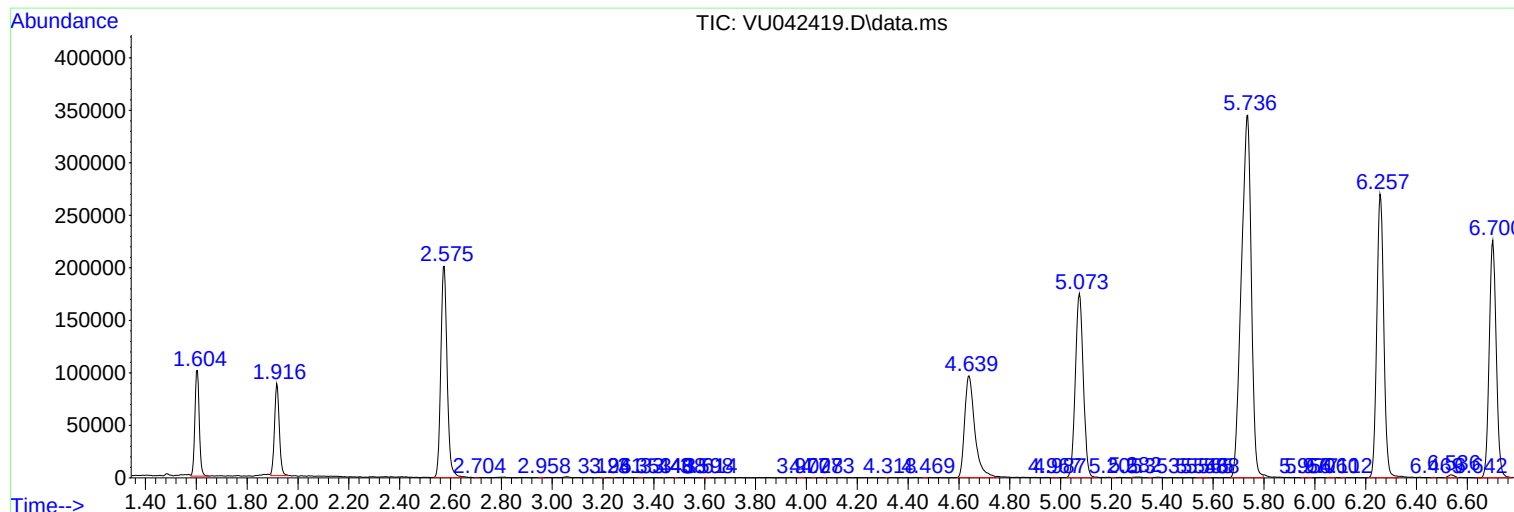

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022421\
Data File : VU042419.D
Acq On : 24 Feb 2021 10:29
Operator : SY/MD
Sample : VU0224WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022421\
Data File : VU042419.D
Acq On : 24 Feb 2021 10:29
Operator : SY/MD
Sample : VU0224WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
