

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022422\
 Data File : VU047259.D
 Acq On : 24 Feb 2022 13:08
 Operator : SY/MD
 Sample : VU0224WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Quant Time: Feb 25 02:04:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM022422.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Feb 25 02:01:23 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.207	114	9990	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.361	117	9240	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.742	152	5727	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.606	65	4143	0.485	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	96.000%		
4) 1,2-Dichloroethane-d4	5.661	65	4304	0.433	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	86.000%		
7) 1,2-Dichloropropane-d6	6.639	67	4379	0.505	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	102.000%		
8) Toluene-d8	7.845	98	11373	0.481	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	96.000%		
10) 1,1,2,2-Tetrachloroeth...	10.679	84	3633	0.491	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	98.000%		
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.684	75	59	0.046	ug/L	Qvalue 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022422\
Data File : VU047259.D
Acq On : 24 Feb 2022 13:08
Operator : SY/MD
Sample : VU0224WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Feb 25 02:04:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM022422.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Feb 25 02:01:23 2022
Response via : Initial Calibration

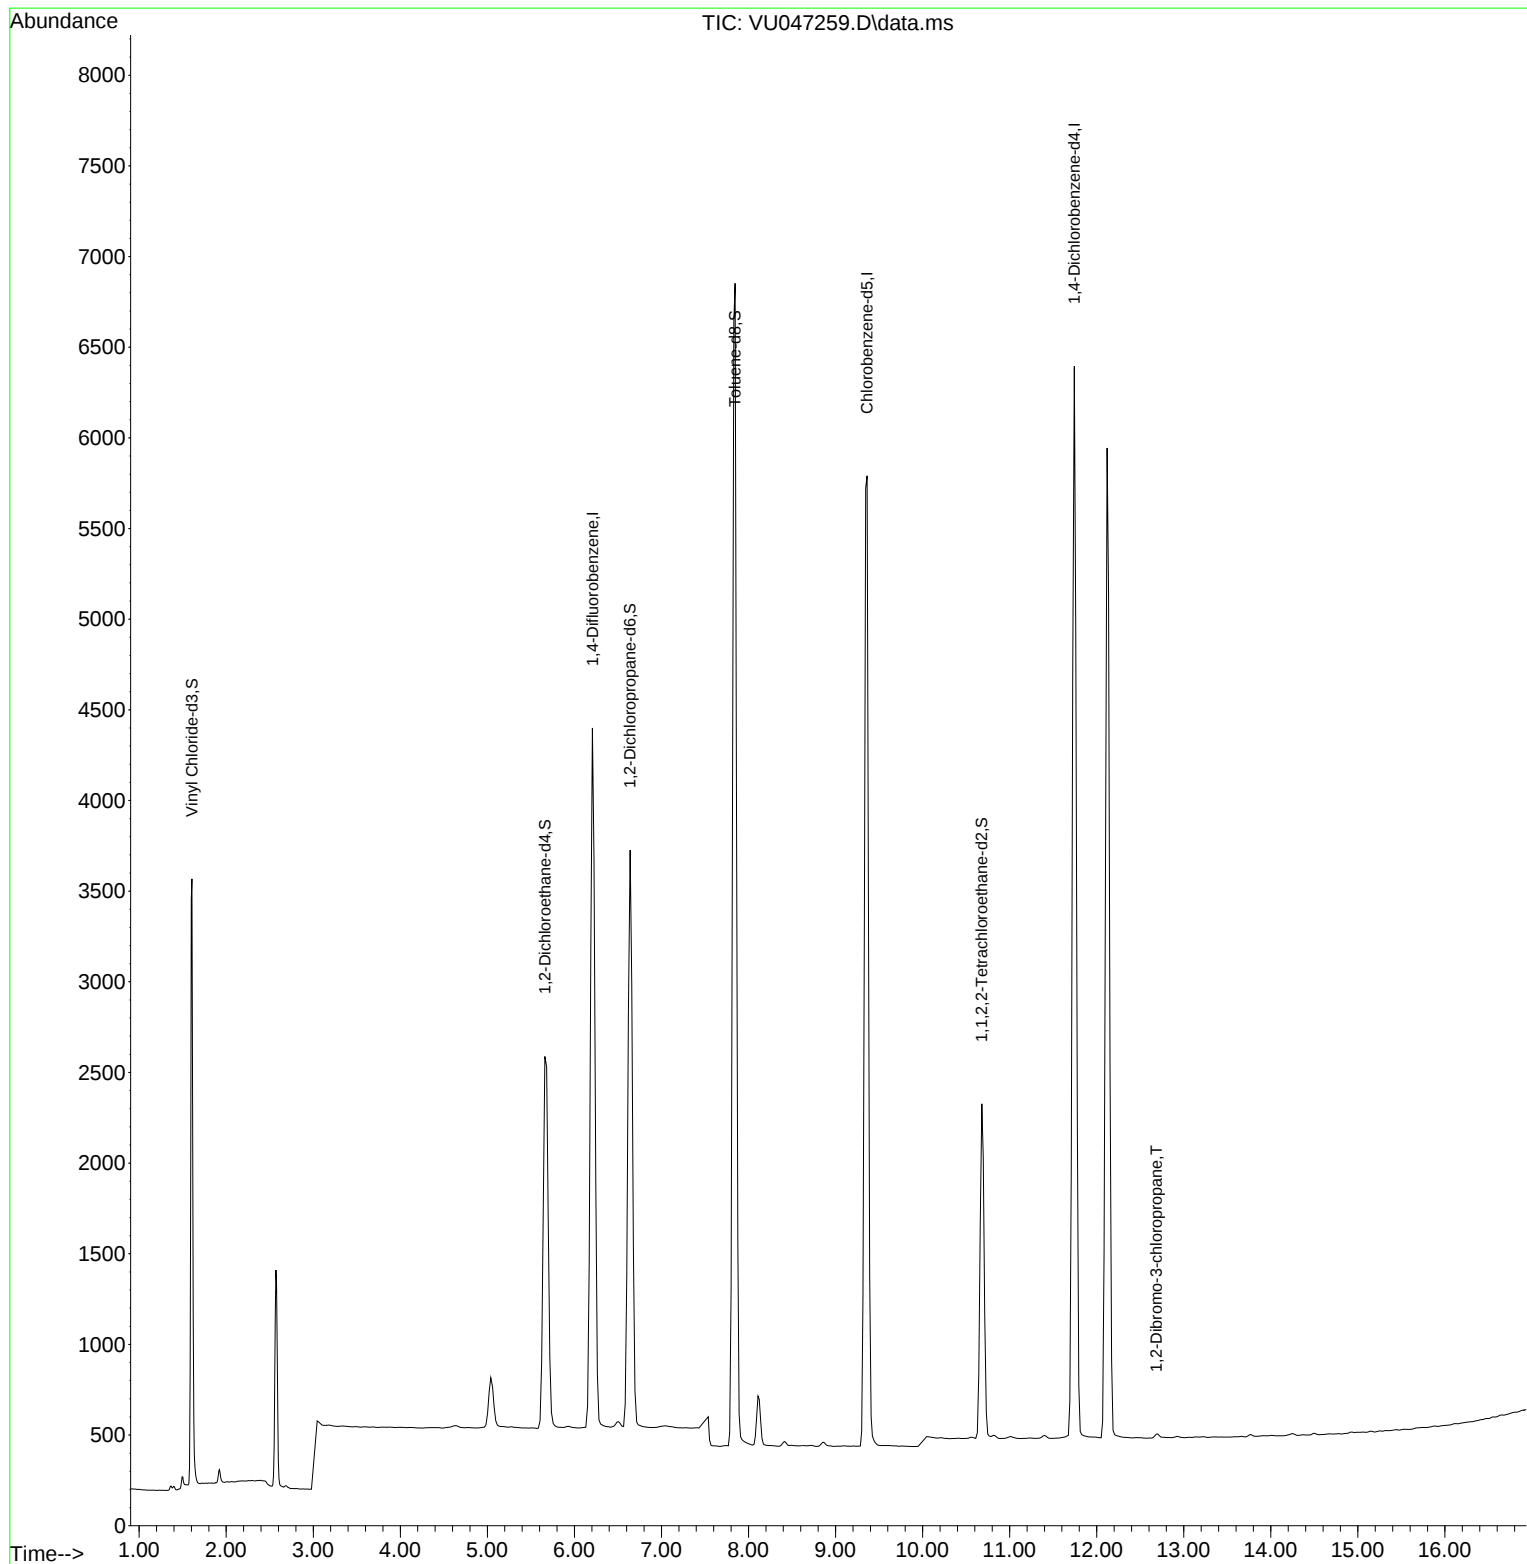

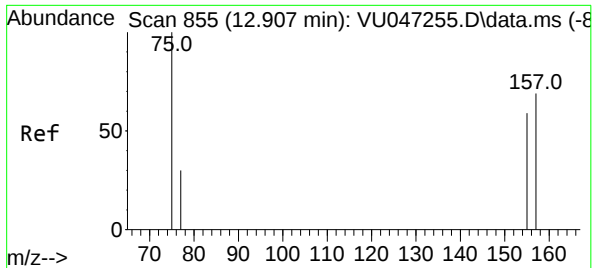

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.046 ug/L
 RT: 12.684 min Scan# 842
 Delta R.T. -0.223 min
 Lab File: VU047259.D
 Acq: 24 Feb 2022 13:08

Tgt Ion: 75	Resp:	59
Ion Ratio	Lower	Upper
75	100	
157	67.6	59.4 89.2
155	70.6	52.7 79.1

