


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022519\
 Data File : VU029645.D
 Acq On : 25 Feb 2019 09:01
 Operator : JC/SP
 Sample : BFB49
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB49

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM021519WMA.M
 Title : VOC Analysis
 Last Update : Tue Feb 26 00:12:24 2019

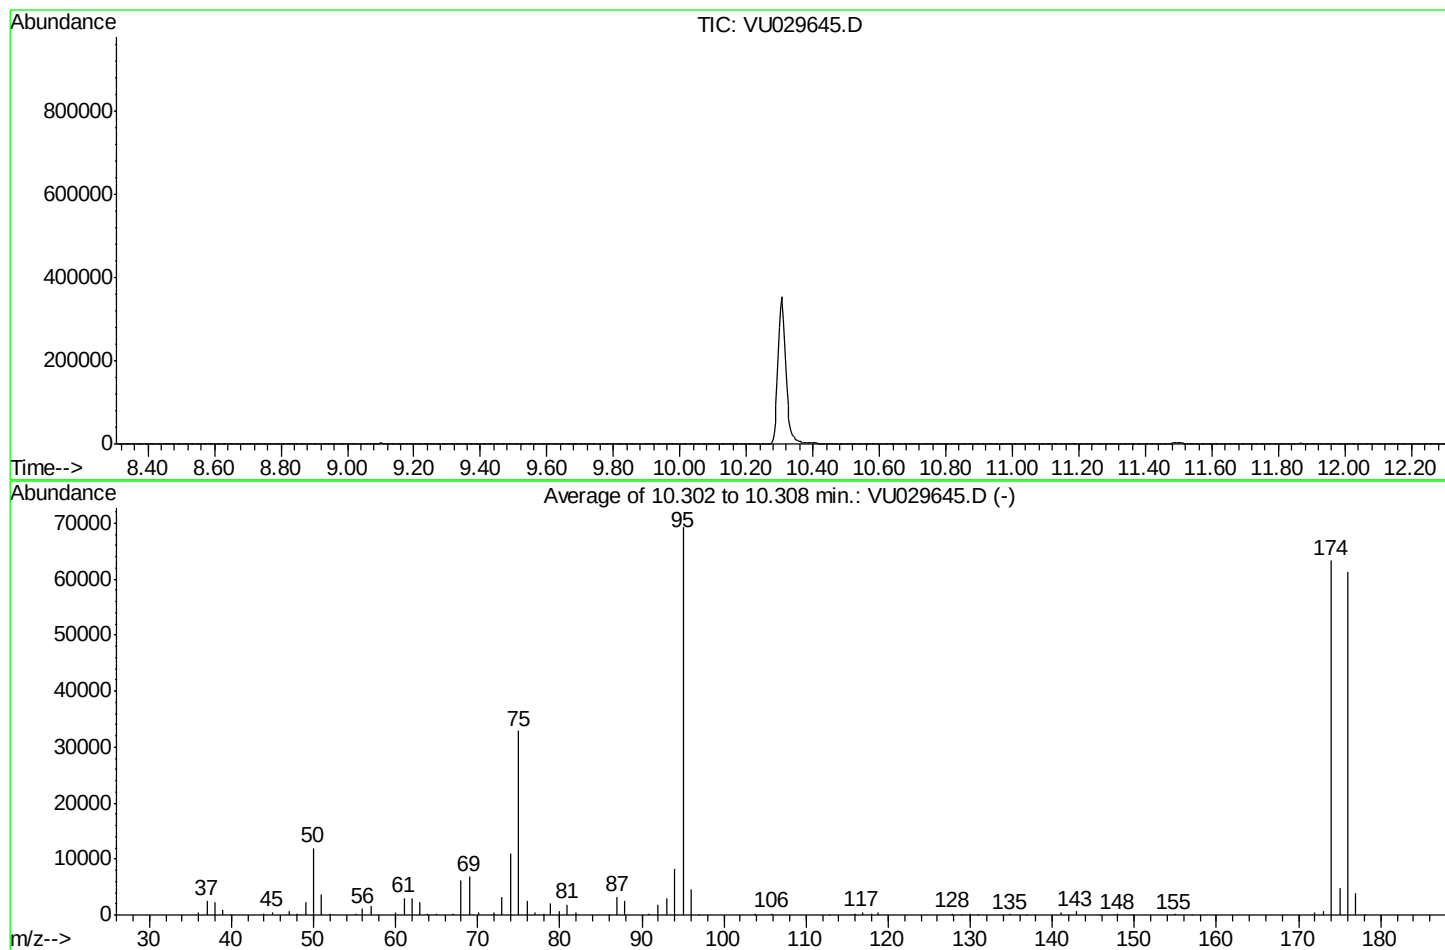

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	11920	PASS
75	95	30	80	47.4	32858	PASS
95	95	100	100	100.0	69266	PASS
96	95	5	9	6.6	4537	PASS
173	174	0.00	2	1.0	655	PASS
174	95	50	120	91.3	63272	PASS
175	174	5	9	7.5	4724	PASS
176	174	95	101	97.0	61392	PASS
177	176	5	9	6.5	3962	PASS

m/z	Abundance
36.00	500.0
37.00	2644.0
38.00	2362.0
39.00	944.0
39.90	191.0
44.00	758.0
45.00	517.0
47.00	689.0
47.90	295.0
49.00	2378.0
50.00	11861.0
51.00	3779.0
52.10	192.0
55.10	256.0
56.00	1007.0
57.00	1575.0
60.00	529.0
61.00	3132.0
62.00	2971.0
63.00	2177.0
64.00	233.0
65.00	200.0
66.90	195.0
68.00	6351.0
69.00	6805.0
70.00	489.0
72.00	397.0
73.00	2909.0
74.00	10518.0
75.00	32400.0
76.10	2714.0
77.00	518.0
78.00	344.0
78.90	2021.0
80.00	711.0
80.90	1769.0
81.90	411.0
86.00	115.0
87.00	2940.0
87.90	2517.0
90.90	218.0
92.00	1723.0
93.00	2908.0
94.00	7801.0
95.00	66832.0
96.00	4513.0
96.90	147.0
103.90	338.0
105.90	311.0
112.80	122.0
115.90	198.0
116.90	531.0
117.90	227.0
118.80	346.0
127.80	265.0
129.90	257.0
131.00	134.0
134.80	187.0
136.80	101.0
141.00	460.0
142.90	723.0
147.90	236.0
149.80	118.0
154.90	183.0
172.00	400.0
173.20	726.0
174.00	59576.0
175.00	4642.0
176.00	58328.0
177.00	4002.0
207.10	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
36.00	490.0
37.00	2577.0
38.00	2326.0
39.00	971.0
39.90	187.0
44.00	812.0
45.00	516.0
47.10	577.0
48.00	318.0
49.00	2430.0
50.00	12427.0
51.00	3756.0
52.10	150.0
55.10	233.0
56.00	1126.0
57.00	1628.0
60.00	566.0
61.00	3185.0
62.00	3044.0
63.00	2417.0
64.00	217.0
65.00	207.0
66.90	203.0
68.00	6468.0
69.00	7140.0
70.00	537.0
72.00	401.0
73.00	3274.0
74.00	11480.0
75.00	34024.0
76.10	2665.0
77.00	451.0
78.00	341.0
78.90	2117.0
79.90	724.0
80.90	2002.0
82.00	446.0
86.10	141.0
87.00	3450.0
88.00	2727.0
90.90	210.0
92.00	1863.0
93.00	3066.0
94.00	8465.0
95.00	71552.0
96.00	4716.0
96.90	126.0
103.80	327.0
105.90	375.0
112.80	113.0
115.90	183.0
116.90	499.0
117.90	227.0
118.80	450.0
127.90	251.0
128.90	131.0
130.00	243.0
131.00	111.0
134.80	201.0
136.80	110.0
141.00	544.0
142.90	683.0
145.70	115.0
148.00	248.0
154.90	195.0
156.90	132.0
172.00	464.0
173.10	636.0
174.00	65264.0
175.00	4816.0
176.00	63440.0
177.00	4119.0
178.00	116.0
207.00	153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
36.00	499.0
37.00	2554.0
38.00	2146.0
39.00	819.0
40.00	181.0
44.00	839.0
44.90	475.0
47.10	480.0
48.00	321.0
49.00	2245.0
50.00	11472.0
51.00	3392.0
52.10	146.0
55.10	168.0
56.00	1078.0
57.00	1522.0
60.00	494.0
61.00	2941.0
62.00	2879.0
63.00	2355.0
63.90	207.0
65.00	225.0
67.00	194.0
68.00	5946.0
69.00	6564.0
70.10	564.0
72.00	353.0
73.00	3182.0
74.00	11232.0
75.00	32152.0
76.00	2422.0
76.90	385.0
78.00	290.0
78.90	1908.0
80.00	603.0
80.90	2032.0
82.00	515.0
87.00	3347.0
87.90	2555.0
90.90	214.0
92.00	1941.0
93.00	2863.0
94.00	8258.0
95.00	69416.0
96.00	4382.0
103.80	307.0
105.90	336.0
115.90	175.0
116.90	411.0
118.00	230.0
118.80	503.0
127.90	236.0
129.00	144.0
129.90	246.0
134.90	182.0
136.90	119.0
141.00	627.0
142.90	647.0
145.70	118.0
147.90	188.0
154.90	184.0
156.90	155.0
171.90	455.0
173.00	605.0
174.00	64976.0
175.00	4716.0
176.00	62408.0
177.00	3766.0
178.00	127.0
207.00	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
39.90	175.0
44.00	546.0
206.90	182.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49