

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU022520\
 Data File : VU036903.D
 Acq On : 25 Feb 2020 13:31
 Operator : JC/MD
 Sample : VIBLK41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	97	rVB	150508	153759	15.41%	2.040%
2	1.906	168	176	189	rVB	114413	151075	15.15%	2.004%
3	2.584	374	387	405	rBV	204069	331825	33.27%	4.401%
4	2.713	423	427	431	rVB3	335	248	0.02%	0.003%
5	2.774	442	446	450	rVB2	190	211	0.02%	0.003%
6	2.983	509	511	515	rBV2	220	106	0.01%	0.001%
7	3.073	533	539	549	rVB5	1389	2273	0.23%	0.030%
8	3.385	633	636	638	rBV2	193	153	0.02%	0.002%
9	3.420	643	647	650	rBV2	197	193	0.02%	0.003%
10	3.462	656	660	664	rVB2	208	209	0.02%	0.003%
11	3.485	664	667	670	rBV2	181	146	0.01%	0.002%
12	3.543	681	685	687	rBV2	279	229	0.02%	0.003%
13	3.597	698	702	703	rBV	164	124	0.01%	0.002%
14	3.636	710	714	719	rVB2	246	286	0.03%	0.004%
15	3.671	719	725	730	rBV2	188	224	0.02%	0.003%
16	3.723	737	741	743	rBV	163	140	0.01%	0.002%
17	3.739	743	746	750	rVV2	255	234	0.02%	0.003%
18	3.761	750	753	758	rVB2	159	119	0.01%	0.002%
19	3.784	758	760	763	rBV	200	148	0.01%	0.002%
20	3.816	767	770	775	rBV	265	212	0.02%	0.003%
21	4.096	855	857	860	rVB2	196	108	0.01%	0.001%
22	4.128	863	867	869	rBV	190	166	0.02%	0.002%
23	4.237	897	901	906	rVB2	233	267	0.03%	0.004%
24	4.266	906	910	912	rBV	194	124	0.01%	0.002%
25	4.298	917	920	922	rBV2	171	118	0.01%	0.002%
26	4.356	936	938	941	rBV	175	117	0.01%	0.002%
27	4.375	941	944	949	rVB2	218	205	0.02%	0.003%
28	4.401	949	952	955	rBV	218	134	0.01%	0.002%
29	4.449	965	967	971	rVB2	163	101	0.01%	0.001%
30	4.504	978	984	987	rBV	243	274	0.03%	0.004%
31	4.604	1012	1015	1019	rVB	311	230	0.02%	0.003%
32	4.671	1019	1036	1060	rBV	97906	228110	22.87%	3.026%
33	4.967	1124	1128	1130	rVB2	146	121	0.01%	0.002%
34	5.102	1153	1170	1188	rBV	169580	367045	36.80%	4.869%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU022520\
 Data File : VU036903.D
 Acq On : 25 Feb 2020 13:31
 Operator : JC/MD
 Sample : VIBLK41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

35	5.237	1207	1212	1215	rBV2	212	196	0.02%	0.003%
36	5.276	1219	1224	1229	rVB2	170	221	0.02%	0.003%
37	5.305	1229	1233	1234	rBV2	187	141	0.01%	0.002%
38	5.404	1261	1264	1265	rBV	273	166	0.02%	0.002%
39	5.623	1327	1332	1335	rBV2	183	210	0.02%	0.003%
40	5.761	1353	1375	1395	rBV2	381827	997483	100.00%	13.231%
41	5.928	1424	1427	1428	rBV2	263	182	0.02%	0.002%
42	6.070	1467	1471	1472	rBV	207	145	0.01%	0.002%
43	6.189	1504	1508	1511	rBV2	200	185	0.02%	0.002%
44	6.231	1517	1521	1522	rBV	233	179	0.02%	0.002%
45	6.282	1523	1537	1556	rVV	329240	607846	60.94%	8.063%
46	6.568	1618	1626	1635	rBV6	1941	3697	0.37%	0.049%
47	6.613	1637	1640	1643	rBV2	196	131	0.01%	0.002%
48	6.645	1646	1650	1653	rBV2	197	181	0.02%	0.002%
49	6.723	1660	1674	1692	rBV	234345	453720	45.49%	6.018%
50	6.928	1734	1738	1744	rBV	257	390	0.04%	0.005%
51	7.005	1756	1762	1764	rVB2	146	134	0.01%	0.002%
52	7.047	1773	1775	1779	rVB	226	135	0.01%	0.002%
53	7.118	1794	1797	1800	rBV	115	103	0.01%	0.001%
54	7.214	1822	1827	1834	rVB2	714	636	0.06%	0.008%
55	7.372	1869	1876	1878	rBV	220	195	0.02%	0.003%
56	7.385	1878	1880	1886	rVB	125	97	0.01%	0.001%
57	7.488	1909	1912	1915	rVB	184	112	0.01%	0.001%
58	7.533	1922	1926	1932	rVB2	288	268	0.03%	0.004%
59	7.594	1932	1945	1961	rBV	130285	226671	22.72%	3.007%
60	7.768	1996	1999	2002	rBV2	177	118	0.01%	0.002%
61	7.803	2007	2010	2012	rBV	196	128	0.01%	0.002%
62	7.838	2019	2021	2025	rBV	241	163	0.02%	0.002%
63	7.925	2034	2048	2064	rBV	477184	812797	81.48%	10.781%
64	8.118	2104	2108	2110	rBV	172	156	0.02%	0.002%
65	8.205	2122	2135	2149	rBV	93143	152018	15.24%	2.016%
66	8.308	2164	2167	2169	rBV2	154	124	0.01%	0.002%
67	8.343	2173	2178	2180	rBV2	179	191	0.02%	0.003%
68	8.388	2189	2192	2195	rBV2	158	133	0.01%	0.002%
69	8.494	2222	2225	2226	rBV	204	138	0.01%	0.002%
70	8.523	2232	2234	2239	rVB2	161	115	0.01%	0.002%
71	8.578	2246	2251	2256	rBV	197	184	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU022520\
 Data File : VU036903.D
 Acq On : 25 Feb 2020 13:31
 Operator : JC/MD
 Sample : VIBLK41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

72	8.665	2263	2278	2315	rBV	315288	552021	55.34%	7.322%
73	8.903	2349	2352	2355	rBV	201	95	0.01%	0.001%
74	8.919	2355	2357	2363	rVB	245	176	0.02%	0.002%
75	9.060	2399	2401	2404	rBV2	165	113	0.01%	0.001%
76	9.144	2423	2427	2431	rBV	172	111	0.01%	0.001%
77	9.301	2472	2476	2478	rBV2	191	170	0.02%	0.002%
78	9.369	2495	2497	2499	rVB	206	105	0.01%	0.001%
79	9.439	2506	2519	2549	rBV	450881	746830	74.87%	9.906%
80	9.648	2580	2584	2588	rBV2	256	232	0.02%	0.003%
81	9.726	2604	2608	2611	rVB2	302	246	0.02%	0.003%
82	9.796	2627	2630	2633	rBV	238	185	0.02%	0.002%
83	10.009	2693	2696	2698	rBV	222	110	0.01%	0.001%
84	10.047	2705	2708	2713	rBV	238	193	0.02%	0.003%
85	10.079	2715	2718	2723	rBV2	201	198	0.02%	0.003%
86	10.173	2745	2747	2750	rBV	180	123	0.01%	0.002%
87	10.266	2774	2776	2779	rBV2	189	104	0.01%	0.001%
88	10.558	2864	2867	2869	rVB	203	108	0.01%	0.001%
89	10.578	2869	2873	2876	rVB	229	180	0.02%	0.002%
90	10.636	2887	2891	2893	rVB	177	128	0.01%	0.002%
91	10.655	2894	2897	2902	rBV2	248	264	0.03%	0.004%
92	10.700	2908	2911	2915	rBV	186	121	0.01%	0.002%
93	10.777	2922	2935	2952	rBV	317421	509101	51.04%	6.753%
94	11.063	3019	3024	3025	rBV	187	151	0.02%	0.002%
95	11.227	3072	3075	3080	rVB2	225	195	0.02%	0.003%
96	11.288	3091	3094	3098	rVB2	261	194	0.02%	0.003%
97	11.465	3144	3149	3152	rBV2	510	538	0.05%	0.007%
98	11.828	3250	3262	3280	rBV	371174	601002	60.25%	7.972%
99	12.211	3368	3381	3398	rVB	380787	624728	62.63%	8.287%
100	14.118	3971	3974	3984	rVB3	1990	2482	0.25%	0.033%


Sum of corrected areas: 7538927

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU022520\
Data File : VU036903.D
Acq On : 25 Feb 2020 13:31
Operator : JC/MD
Sample : VIBLK41
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

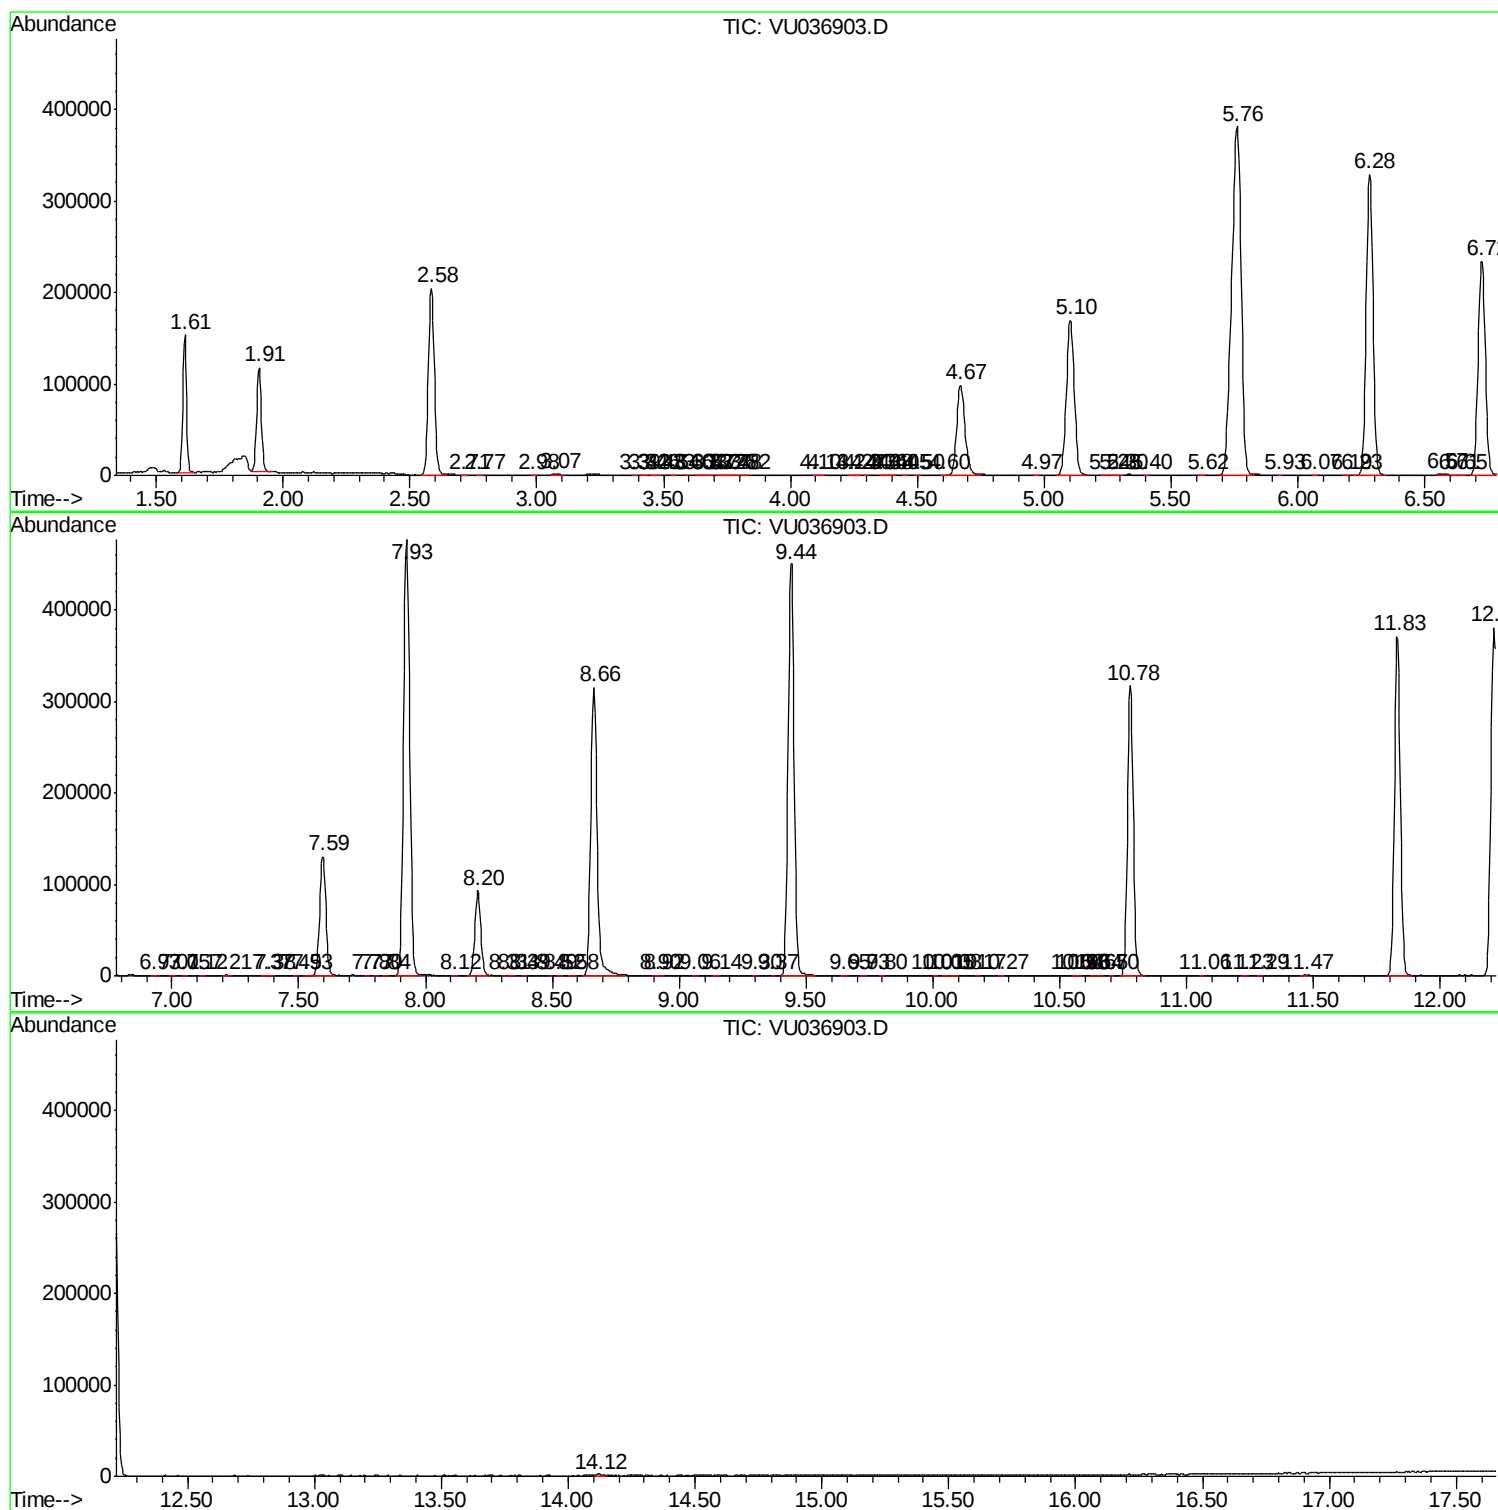

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU022520\
Data File : VU036903.D
Acq On : 25 Feb 2020 13:31
Operator : JC/MD
Sample : VIBLK41
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU022520\
Data File : VU036903.D
Acq On : 25 Feb 2020 13:31
Operator : JC/MD
Sample : VIBLK41
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc