


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU022520\
 Data File : VU036896.D
 Acq On : 25 Feb 2020 09:48
 Operator : JC/MD
 Sample : BFB51
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB51

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis
 Last Update : Wed Feb 26 02:49:26 2020

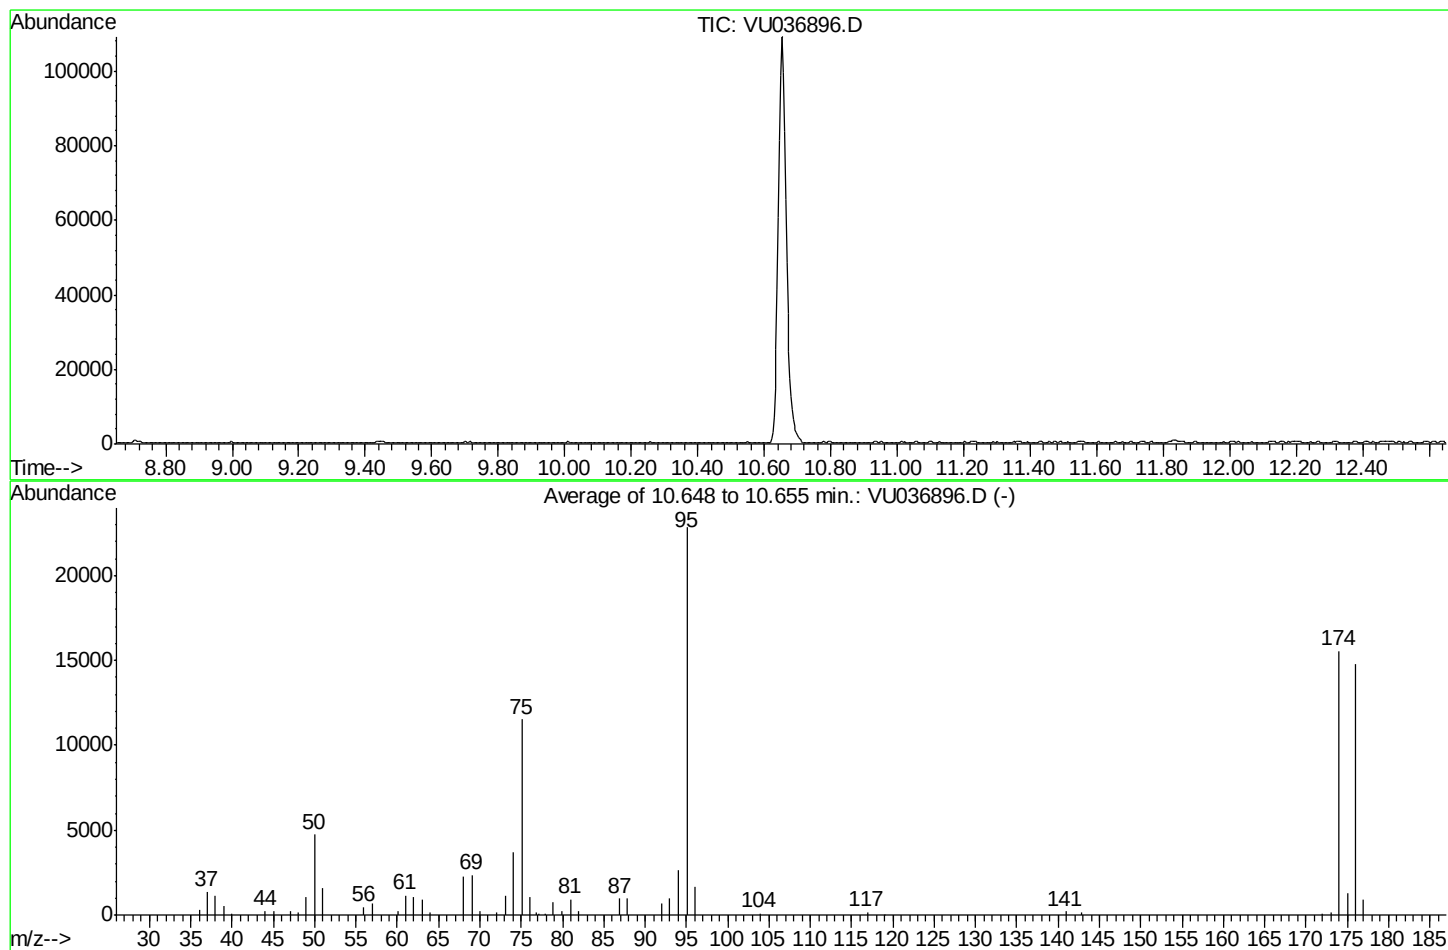

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	4726	PASS
75	95	30	80	50.4	11525	PASS
95	95	100	100	100.0	22850	PASS
96	95	5	9	7.1	1627	PASS
173	174	0.00	2	1.2	179	PASS
174	95	50	120	68.0	15545	PASS
175	174	5	9	8.2	1267	PASS
176	174	95	101	95.2	14801	PASS
177	176	5	9	6.2	911	PASS

m/z	Abundance
36.00	285.0
37.00	1277.0
38.00	1120.0
39.00	509.0
40.00	102.0
44.00	608.0
45.00	182.0
47.10	220.0
48.00	163.0
49.00	1029.0
50.00	4541.0
51.00	1573.0
56.00	450.0
57.00	668.0
60.10	282.0
60.90	1061.0
62.00	1067.0
63.00	867.0
64.00	162.0
68.00	2262.0
69.00	2140.0
70.00	189.0
72.00	159.0
73.10	1052.0
74.10	3784.0
75.00	10688.0
76.10	982.0
76.80	166.0
78.90	717.0
79.90	195.0
81.00	843.0
81.90	207.0
86.90	862.0
87.90	867.0
92.00	563.0
93.00	817.0
94.00	2468.0
95.10	21480.0
96.00	1503.0
116.90	195.0
141.00	200.0
142.90	159.0
172.00	135.0
173.00	252.0
174.00	14504.0
175.00	1224.0
176.00	13416.0
177.00	776.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
36.00	287.0
37.00	1442.0
38.00	1138.0
39.00	558.0
40.00	114.0
44.00	612.0
45.00	221.0
47.10	246.0
48.00	182.0
49.00	1099.0
50.00	4894.0
51.00	1627.0
55.90	506.0
56.90	712.0
60.10	261.0
60.90	1161.0
62.00	1123.0
63.00	954.0
64.00	158.0
68.00	2338.0
69.00	2429.0
70.00	215.0
72.00	150.0
73.10	1151.0
74.00	3813.0
75.00	11815.0
76.10	1120.0
76.90	182.0
77.90	105.0
78.90	784.0
79.90	216.0
80.90	926.0
81.90	218.0
86.90	1001.0
87.90	989.0
92.00	682.0
93.00	1033.0
94.10	2713.0
95.10	23584.0
96.00	1717.0
103.90	109.0
116.90	202.0
140.90	192.0
142.90	150.0
172.00	131.0
173.00	287.0
174.00	16029.0
175.00	1280.0
176.00	15376.0
177.00	928.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
36.00	270.0
37.00	1397.0
38.00	1093.0
39.00	527.0
39.90	111.0
44.00	554.0
45.00	236.0
47.10	276.0
48.00	183.0
49.00	1103.0
50.00	4743.0
51.00	1528.0
55.90	467.0
56.90	679.0
60.10	221.0
61.00	1189.0
62.00	1088.0
63.00	943.0
63.90	129.0
68.00	2299.0
69.00	2555.0
70.10	238.0
72.00	165.0
73.10	1141.0
74.00	3594.0
75.10	12074.0
76.00	1144.0
77.10	192.0
77.90	144.0
78.90	818.0
80.00	271.0
80.90	957.0
81.90	187.0
87.00	1029.0
87.90	1012.0
92.00	741.0
93.00	1120.0
94.10	2764.0
95.10	23488.0
96.00	1662.0
103.90	130.0
116.90	165.0
118.90	102.0
140.90	207.0
142.90	158.0
174.00	16104.0
175.00	1299.0
176.00	15613.0
177.00	1029.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
44.00	353.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51