

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022521\
 Data File : VU042433.D
 Acq On : 25 Feb 2021 16:43
 Operator : SY/MD
 Sample : VU0225WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK204

Quant Time: Feb 26 06:25:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM022521.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Feb 26 06:20:15 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.225	114	3947	0.50	ug/L	0.00
5) Chlorobenzene-d5	9.364	117	3482	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.745	152	1920	0.50	ug/L	-0.01
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.605	65	1567	0.51	ug/L	0.00
Spiked Amount	0.500	Range 40 - 130	Recovery	=	102.00%	
4) 1,2-Dichloroethane-d4	5.679	65	1856	0.46	ug/L	0.00
Spiked Amount	0.500	Range 70 - 130	Recovery	=	92.00%	
7) 1,2-Dichloropropane-d6	6.658	67	1632	0.53	ug/L	0.00
Spiked Amount	0.500	Range 60 - 140	Recovery	=	106.00%	
8) Toluene-d8	7.848	98	4313	0.49	ug/L	0.00
Spiked Amount	0.500	Range 70 - 130	Recovery	=	98.00%	
10) 1,1,2,2-Tetrachloroeth...	10.682	84	1354	0.52	ug/L	-0.01
Spiked Amount	0.500	Range 65 - 120	Recovery	=	104.00%	
Target Compounds						Qvalue
13) 1,2-Dibromo-3-chloropr...	12.704	75	9	0.02	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022521\
Data File : VU042433.D
Acq On : 25 Feb 2021 16:43
Operator : SY/MD
Sample : VU0225WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK204


Quant Time: Feb 26 06:25:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM022521.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Feb 26 06:20:15 2021
Response via : Initial Calibration

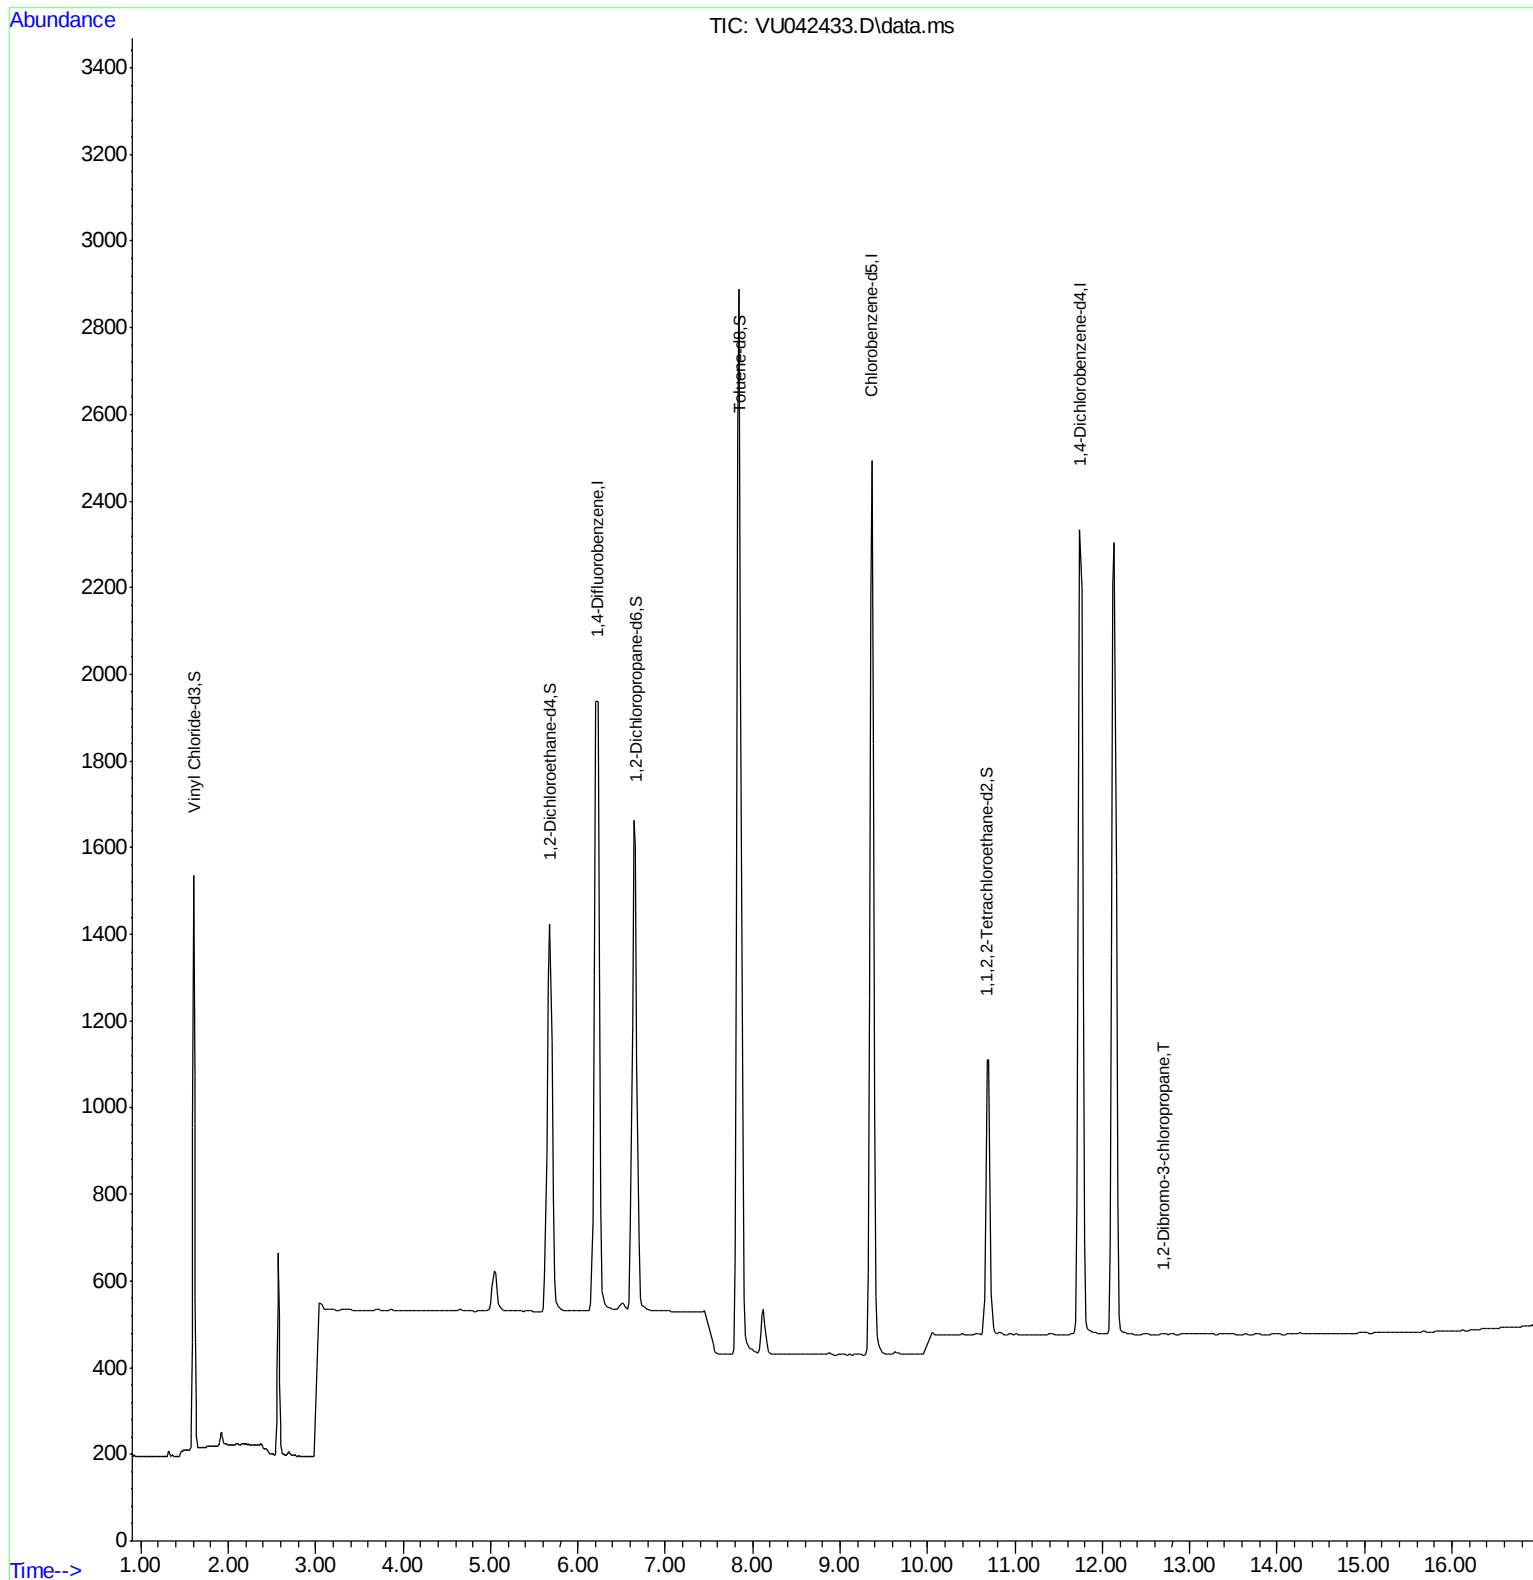

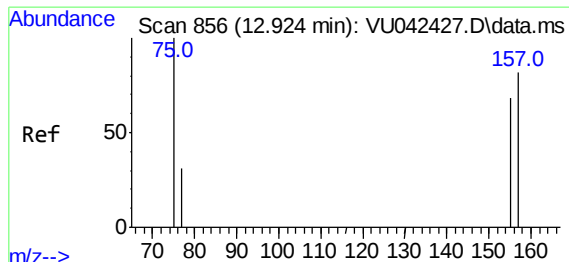

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.02 ug/L
 RT: 12.704 min Scan# 843
 Delta R.T. -0.220 min
 Lab File: VU042433.D
 Acq: 25 Feb 2021 16:43

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK204

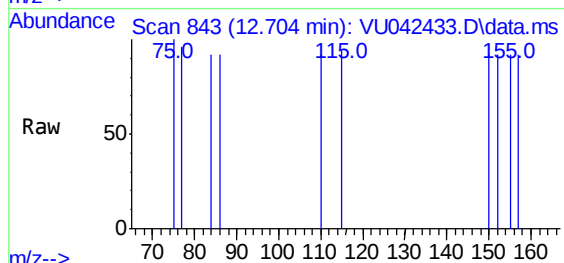

Tgt Ion: 75 Resp: 9
 Ion Ratio Lower Upper
 75 100
 157 92.2 70.2 105.2
 155 92.2 63.0 94.4

